

- (21) Application No 8319148
- (22) Date of filing 15 Jul 1983
- (30) Priority data
- (31) 8223115
- (32) 11 Aug 1982
- (33) United Kingdom (GB)
- (43) Application published 7 Mar 1984
- (51) INT CL<sup>3</sup>  
G01F 1/62
- (52) Domestic classification  
G1N 19B2R 19H2B 512  
522 523 524 525 527 534  
545 582  
U1S 2150 G1N
- (56) Documents cited  
None
- (58) Field of search  
G1N
- (71) Applicants  
Picker International  
Limited  
(United Kingdom),  
East Lane,  
Wembley,  
Middlesex
- (72) Inventors  
Michael Burl  
Ian Robert Young
- (74) Agent and/or  
Address for Service  
M. B. W. Pope,  
Central Patent  
Department,  
(Wembley Office),  
The General Electric  
Company plc,  
Hirst Research Centre,  
East Lane,  
Wembley,  
Middlesex

(54) Nuclear magnetic resonance method and apparatus

(57) A method and apparatus for determining the rate of flow of a liquid in a selected region of a body by nuclear magnetic resonance techniques. The method includes a sequence of applying a first magnetic pulse ( $B_1(90^\circ)$ ) effective to excite nuclear magnetic resonance of a chosen nucleus within the liquid preferentially in a slice of the body which includes the selected region. A period of time ( $t_D$ ) is waited and then a second magnetic pulse ( $B_1(90^\circ)$ ) is applied which is effective to excite nuclear magnetic resonance of the nuclei preferentially in the slice, and the free induction decay signal is measured. The whole sequence is repeated for different values of the period of time ( $t_D$ ). The variation in the value of the measured signal with  $t_D$  is then related to the rate of flow of the liquid through the slice.

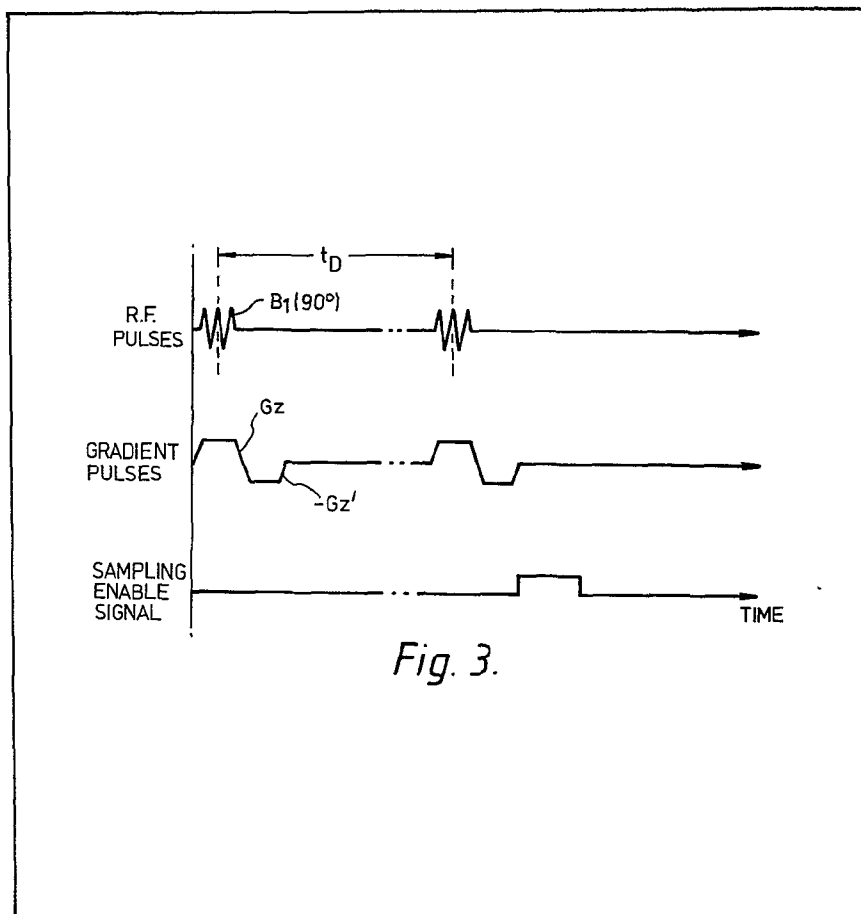


Fig. 3.

Fig. 1.

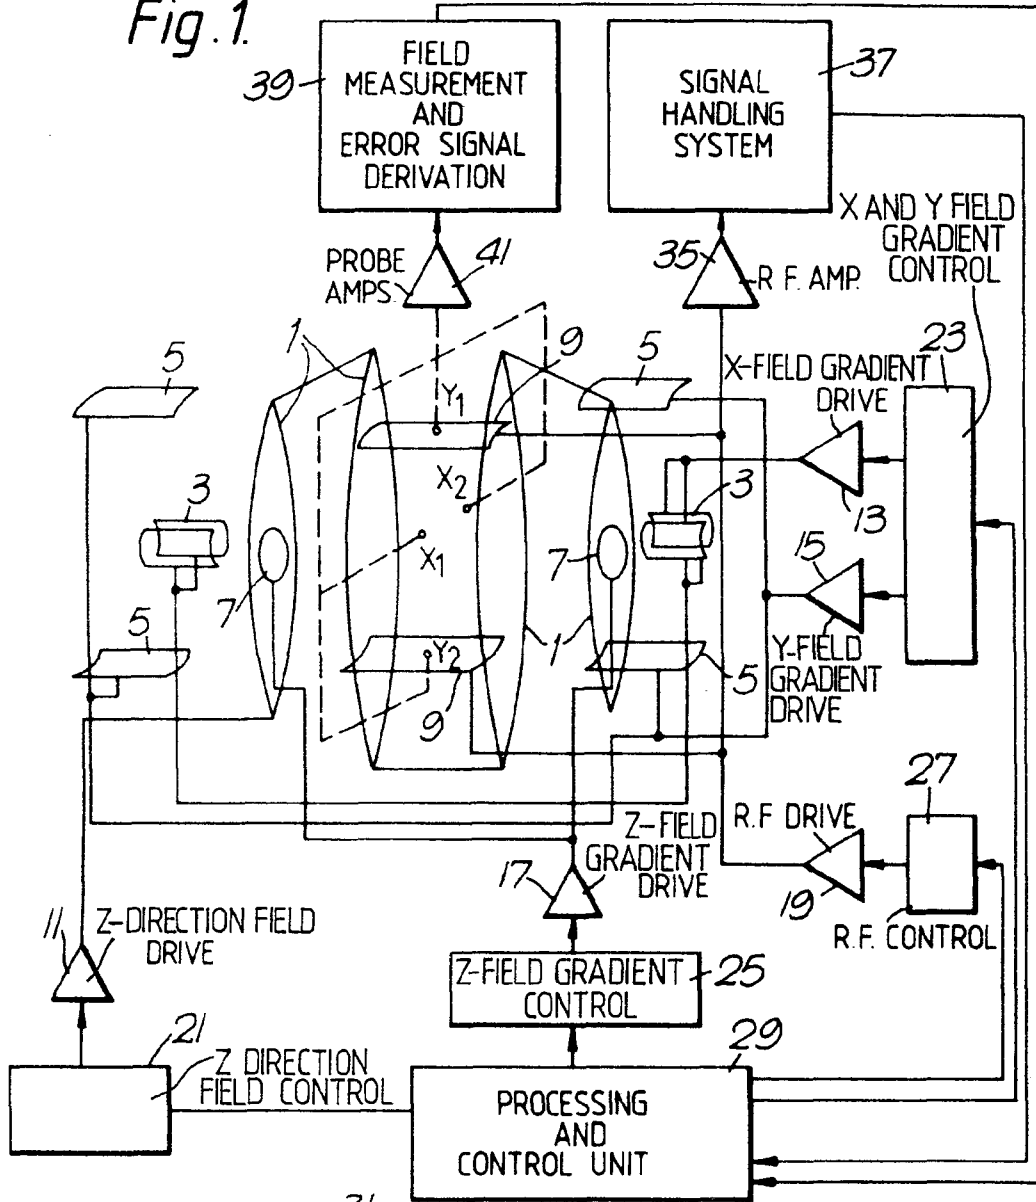
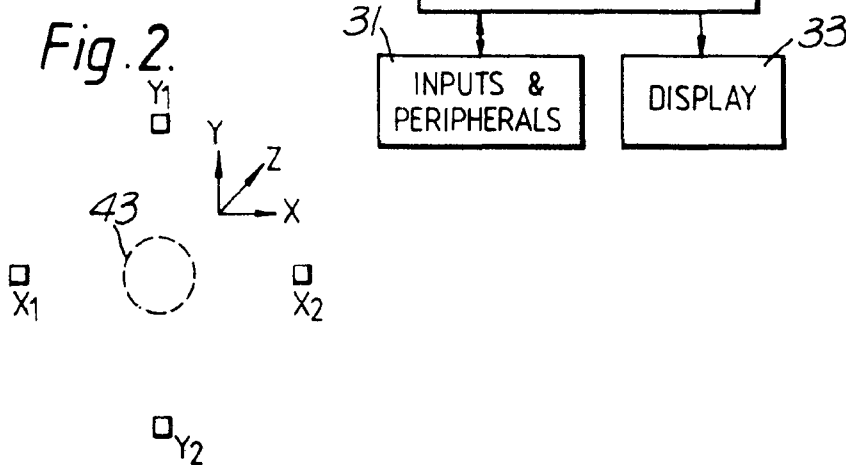


Fig. 2.



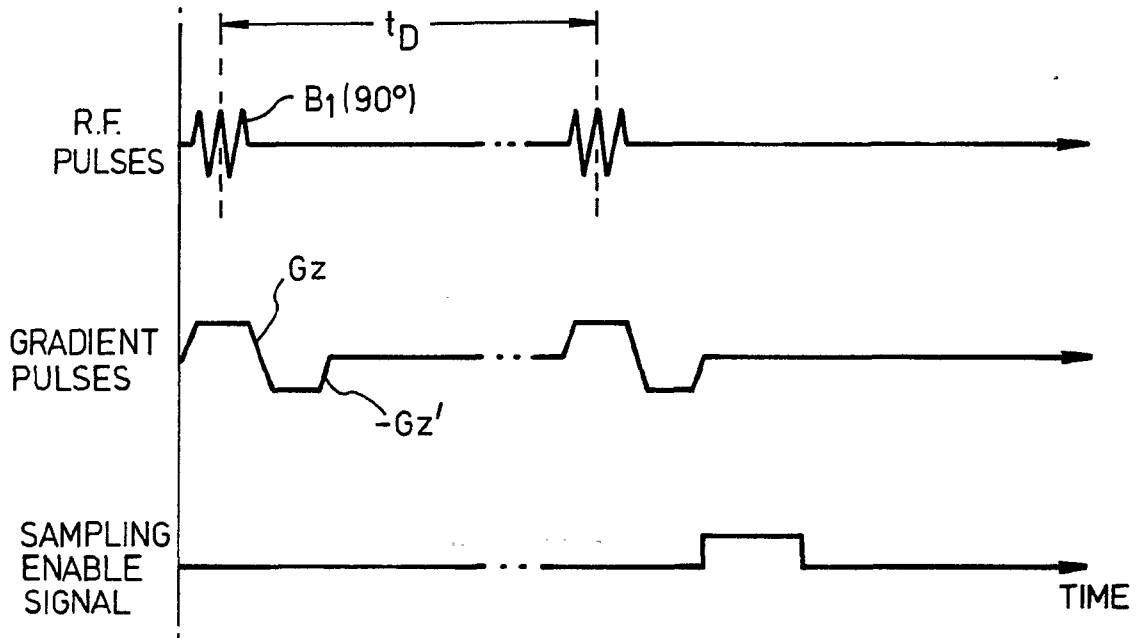


Fig. 3.

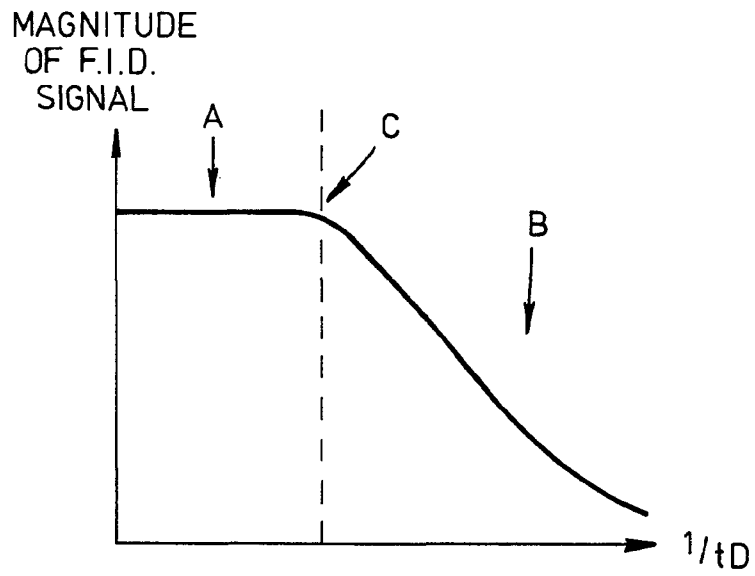


Fig. 4.

## SPECIFICATION

**Nuclear magnetic resonance method and apparatus**

5 This invention relates to methods and apparatus for determining the rate of flow of a liquid in a selected region of a body by nuclear magnetic resonance (NMR) techniques.

10 NMR techniques have been used for the chemical analysis of material for many years. More recently NMR techniques have been used to obtain images representing the distribution over a selected cross-sectional slice or volume of a body of a chosen quantity, e.g. the density of chosen nuclei, for  
 15 *example hydrogen protons, or of NMR spin relaxation time constants. Such distributions are similar to, although of different significance from, the distributions of X-ray attenuation provided by computerised tomography systems. In some applications it would*  
 20 *be useful to obtain additional information relating to the flow rates of a liquid within a selected region of the body, e.g. blood flow in selected veins and arteries of a human body, using NMR techniques.*

25 It is an object of the invention to provide a method of determining the rate of flow of a liquid in a selected region of a body by NMR techniques.

According to the present invention a method of determining the rate of flow of a liquid including a chosen nucleus in a region of a body comprises:  
 30 sequentially applying a first magnetic pulse effective to excite nuclear magnetic resonance of said nuclei preferentially in a slice of said body which includes said region, waiting a period of time and then applying a second magnetic pulse effective to excite nuclear  
 35 magnetic resonance of said nuclei preferentially in said slice and measuring the free induction decay signal; repeating said sequence for different values of said period of time; and relating the values of said period of time and the corresponding measured  
 40 signals to the rate of flow of said liquid through said slice.

The invention also provides an apparatus arranged to carry out a method according to the invention, including means arranged to sequentially apply a first  
 45 magnetic pulse effective to excite nuclear magnetic resonance of said nuclei preferentially in a slice of said body which includes said region, wait a period of time and then apply a second magnetic pulse effective to excite nuclear magnetic resonance of said nuclei  
 50 preferentially in said slice and measure the free induction decay signal and repeat said sequence for different values of said period of time.

One method and apparatus in accordance with the invention will now be described, by way of example  
 55 only with reference to the accompanying drawings in which:

Figures 1 and 2 illustrate the apparatus diagrammatically;

60 Figure 3 illustrates the magnetic field sequence employed in the method; and

Figure 4 is a graphical illustration of the relationship between the measured free induction decay signal

and the repetition rate of the magnetic field sequence.

The method is performed using an apparatus  
 65 essentially identical to that described in U.K. Patent Specification No. 1,578,910 or No. 2,056,078, to which reference should be made for a fuller description, appropriately programmed to apply a sequence of magnetic field gradient and R.F. pulses and analyse  
 70 the resulting signals as hereafter described.

The essential features of such an apparatus in so far as is required for an understanding of the present invention are as follows:

The apparatus includes a first coil system whereby a  
 75 magnetic field can be applied to a body to examine in a given direction, normally designated the Z-direction, with a gradient in any one or more of the three orthogonal directions i.e. X, Y and Z directions.

Referring to Figure 1, the first coil system comprises  
 80 coils 1 capable of providing a steady uniform magnetic field in the Z direction; coils 3 capable of providing a magnetic field gradient in the X direction, coils 5 capable of providing a magnetic field gradient in the Y direction; and coils 7 capable of providing a magnetic  
 85 field gradient in the Z direction.

In addition, the apparatus includes a second coil system 9 whereby RF magnetic fields can be applied to the body under examination in a plane normal to the direction of the steady uniform magnetic field produced by the first coil system, and whereby RF  
 90 magnetic fields resulting from nuclei in the body under examination which have been excited to nuclear magnetic resonance with a spin vector component other than in the Z direction can be detected.

In the drawing a single pair of coils 9 is shown for both applying and detecting RF fields, but in certain  
 95 circumstances it may be preferable to provide separate coils for detecting the RF fields.

The various coils 1, 3, 5, 7 and 9 are driven by drive  
 100 amplifiers 11, 12, 13, 15, 17 and 19 respectively, controlled by control circuits 21, 23, 25 and 27 respectively. These circuits may take various forms which are well known to those with experience of NMR equipment and other apparatus using coil  
 105 induced magnetic fields.

The circuits 21, 23, 25 and 27 are controlled by a central processing and control unit 29 with which are associated inputs and other peripherals 31, for the provision of commands and instructions to the  
 110 apparatus, and a display 33.

The NMR signals detected by the coils 9 are applied via an amplifier 35 to a signal handling system 37. The signal handling system is arranged to make any appropriate calibration and correction of the signals, but essentially transmits the signals to the processing  
 115 and control unit 29 wherein the signals are processed for application to the display to produce an image representing the distribution of an NMR quantity in the body being examined.

120 It will be appreciated that whilst shown separately to clarify the present description, the signal handling system 37 may conveniently form part of the unit 29.

The apparatus also includes field measurement and error signal circuits 39 which receive signals via

amplifiers 41 from field probes  $X_1, X_2, Y_1$  and  $Y_2$  which are disposed at suitable positions in relation to a slice 43 of the body being examined, as illustrated in Figure 2, to monitor the applied magnetic fields.

5 Referring now also to Figure 3, in operation of the apparatus a steady uniform magnetic field  $B_0$  is applied to the body under examination in the Z direction. The field serves to define the equilibrium axis of magnetic alignment of the nuclei in the body 10 i.e. along the Z direction, and remains constant throughout the examination procedure. A magnetic field gradient  $G_z$  along the Z direction is then applied to the body, together with an RF magnetic field pulse denoted  $B_1$  ( $90^\circ$ ), for reasons explaining hereafter. The 15 frequency of the RF field is chosen to be the Larmor frequency for hydrogen protons in a slice 43 of the body, normal to the Z direction, the slice being defined by a particular magnetic field along the Z direction, such that hydrogen protons within the slice are 20 preferentially excited, the slice consisting of an area of substantially solid material through which a series of blood vessels extend. The integral of the RF pulse is such that the pulse is just sufficient to tip the spins of the excited protons into the X-Y plane, and is thus 25 referred to as a  $90^\circ$  pulse, the spins then precessing in the X-Y plane round the Z axis.

The field gradient  $G_z$  is then removed, and replaced by a field gradient in the opposite sense —  $G_z'$ . This causes the rephasing of the spins which have been 30 selectively excited by the combination of the RF pulse  $B_1$  ( $90^\circ$ ),  $B_0$  and the field gradient  $G_z$  the dephasing having been caused by the gradient through the slice. The magnitude of —  $G_z'$  is adjusted so that the spins are rephased at the time at which this field gradient is 35 switched of as described, for example, in the above mentioned U.K. Patent Specification No. 1,578,910.

After a time  $t_D$  has elapsed since the pulse  $B_1$  ( $90^\circ$ ), a second  $B_1$  ( $90^\circ$ ) pulse is applied together with the field gradient  $G_z$ , this again being followed by the field 40 gradient —  $G_z'$ . The signal induced in the second coil system 9 by the excited protons in the slice, i.e. the free induction decay (F.I.D.) signal is then recorded. This double excitation sequence is then repeated a number of times with the time  $t_D$  between the successive 45 excitation pulses  $B_1$  ( $90^\circ$ ) being varied through a range of values.

Referring now also to Figure 4, a graph is plotted of the magnitude of the F.I.D. signals measured, i.e. an indication of the density of the excited nuclei within 50 the slice, against the excitation pulse repetition frequency,  $1/t_D$ . As  $t_D$  is always chosen to be much shorter than the spin-lattice relaxation time  $T_1$  for hydrogen protons within the slice, the excited nuclei do not have time to relax back to their equilibrium spin 55 orientation along the Z direction. Thus the second  $B_1$  ( $90^\circ$ ) pulse will remove spins remaining in the X-Y plane into the — Z direction, these spins then not contributing to the measured F.I.D. signal. In the case of blood within the vessels in the slice however, blood 60 which was initially in the slice during the first  $B_1$  ( $90^\circ$ ) pulse, and has subsequently flowed out of the slice during the period  $t_D$ , is replaced by fresh blood having unexcited hydrogen protons prior to the second  $B_1$  ( $90^\circ$ ) pulse. Thus after excitation by the second  $B_1$  ( $90^\circ$ ) 65 pulse, these 'fresh blood' spins contribute to the F.I.D.

measured. For long values of  $t_D$ , i.e. a low excitation pulse repetition rate  $1/t_D$ , the blood has time to be completely replaced within the slice, and thus the plateau region A of the graph shown in Figure 4 is 70 achieved. As the excitation pulse repetition rate  $1/t_D$  increases, however, the blood does not have time to be completely replaced, and thus after a certain value of  $1/t_D$  the FID signal begins to decrease with a further increase in  $1/t_D$  as shown in region B of the graph. The 75 shoulder C indicated on the graph at the cross-over point between the regions A and B thus gives an indication of the minimum time period during which blood is completely replaced within the slice, and from this the flow rate of the blood through the vessels in 80 the slice can be calculated.

It is found that this method is suitable for measuring flow rates for blood which is replaced within a slice in the time range 0.1 to 1.0 seconds.

In the double excitation sequence described herebefore, the F.I.D. signal is not recorded after the first 85 excitation pulse  $B_1$  ( $90^\circ$ ) in each sequence. It will be appreciated however that in a continuous repetition of this sequence it may be more convenient to record the F.I.D. signal after the second excitation pulse and then 90 after each subsequent excitation pulse, with  $t_D$  being the interval between successive excitation pulses. A correction to the measured F.I.D.s will then have to be made to compensate for spins which are not aligned along the equilibrium direction Z during the first 95 excitation pulse in each pair of pulses.

It will also be appreciated that within each repetition time  $t_D$  known NMR techniques using magnetic fields 100 gradients in the X and Y directions may be employed in order to obtain information relating to the spatial distribution over the chosen slice of quantities relating to nuclear magnetic resonance, e.g. the density of a nucleus, or NMR spin relaxation time constants.

It will be appreciated that whilst the method described herebefore relates to obtaining the flow rate 105 of a liquid which includes hydrogen protons, the method is equally applicable to obtaining the flow rate of a liquid including any other nucleus having a spin, e.g.  $^{31}\text{P}$ , by appropriate choice of the R.F. pulse frequency.

## 110 CLAIMS

1. A method of determining the rate of flow of a liquid including a chosen nucleus in a region of a body comprising: sequentially applying a first magnetic pulse effective to excite nuclear magnetic resonance 115 of said nuclei preferentially in a slice of said body which includes said region, waiting a period of time and then applying a second magnetic pulse effective to excite nuclear magnetic resonance of said nuclei preferentially in said slice and measuring the free induction decay signal; repeating said sequence for 120 different values of said period of time; and relating the values of said period of time and the corresponding measured signals to the rate of flow of said liquid through said slice.

2. A method according to Claim 1 in which said first and second magnetic pulses are each sufficient to rotate the spins of said nuclei through an angle of substantially  $90^\circ$ .

3. A method according to either of the preceding 130 claims in which said free induction decay signal is

measured after said second magnetic pulse, and then after each subsequent magnetic pulse.

4. A method according to any one of the preceding claims in which nuclear magnetic resonance imaging techniques are employed during said period of time in order to obtain information relating to the spatial distribution over said slice of quantities relating to nuclear magnetic resonance.

5. A method according to any one of the preceding claims in which said relating comprises determining the minimum value of said time period which is sufficient for said liquid to be completely replaced in said slice by the time of the next excitation.

6. A method according to claim 5 in which said relating comprises determining the reciprocal of the value of said period of time at which said measured signal begins to decrease for increasing values of the reciprocal of the values of said period of time.

7. A method of determining the rate of flow of a liquid including a chosen nucleus in a region of a body, substantially as hereinbefore described with reference to the accompanying drawings.

8. An apparatus arranged to determine the rate of flow of a liquid including a chosen nucleus in a region of a body including: means arranged to sequentially apply a first magnetic pulse effective to excite nuclear magnetic resonance of said nuclei preferentially in a slice of said body which includes said region, wait a period of time and then apply a second magnetic pulse effective to excite nuclear magnetic resonance of said nuclei preferentially in said slice and measure the free induction decay signal and repeat said sequence for different values of said period of time.

9. An apparatus arranged to determine the rate of flow of liquid including a chosen nucleus in a region of a body, substantially as hereinbefore described with reference to the accompanying drawings.