

Conf-9310195-2

Alpha Particle Collective Thomson Scattering in TFTR

John S. Machuzak, Paul P. Woskov, David Y. Rhee and
James Gilmore
*Massachusetts Institute of Technology, Plasma Fusion Center, Cambridge, MA
02139*

Norton L. Bretz and Hyeon K. Park
*Princeton University Plasma Physics Laboratory, James Forrestal Campus,
P.O. Box 451, Princeton, NJ 08544*

Richard E. Aamodt, Peter Y. Cheung and David A. Russell
Lodestar Research Corporation, 2400 Central Ave, P-5, Boulder, CO 80301

Henrik Bindslev
JET Joint Undertaking, Abingdon, Oxon, OX14 3EA, UK

RECEIVED
NOV 19 1993
OSTI

A collective Thomson scattering diagnostic is being implemented on TFTR to measure alpha particle, energetic and thermal ion densities and velocity distributions. A 60 GHz, 0.1-1 kW gyrotron will be used as the transmitter source, and the scattering geometry will be perpendicular to the magnetic field in the extraordinary mode polarization. An enhanced scattered signal is anticipated from fluctuations in the lower hybrid frequency range with this scattering geometry. Millimeter wave collective Thomson scattering diagnostics have the advantage of larger scattering angles to decrease the amount of stray light, and long, high power, modulated pulses to obtain improved signal to noise through synchronous detection techniques.

I. INTRODUCTION

Collective Thomson scattering[1,2] has been traditionally used for measuring the ion species and ion temperature in the earth's ionosphere[3,4], and in many laboratory plasmas[4-11]. The detected signal is due to the scattering of the electromagnetic radiation by the Debye cloud of electrons which effectively surround each ion. These clouds of electrons move with the ions and impart a Doppler shift to the detected scattered radiation which provides a signature of the ion velocity distribution. In tokamaks, very high power and long wavelengths are required to see the collective Thomson scattered ion feature[11]. In order to measure the much smaller (approximately 0.1 - 1%) alpha ion fraction, many proposals have relied on high power, long pulse sources using wavelengths near the plasma cut off frequencies. The large Doppler shift of the alpha particles, which are born at 3.5 MeV energy, is used to distinguish the alpha particles from other plasma ions. These ideas required extensions of the scattering theory to situations

MASTER

DISTRIBUTION OF THIS DOCUMENT IS UNLIMITED

dk

where the scattering frequency is approximately the electron plasma frequency[12,13] and where transverse components of the dielectric tensor are required to describe the dielectric shielding[14,15].

II. EXPERIMENTAL ARRANGEMENT

The type of collective Thomson scattering to be implemented on TFTR differs from previous proposed experiments in that it will make use of a scattering resonance achieved when the fluctuations' wave vectors and frequencies are in the vicinity of weakly damped plasma waves. In this case, the fluctuations are near the lower hybrid frequency[16,17]. For this experiment, a 0.1 to 1 kW, modulated 60 GHz gyrotron is pulsed for up to 1 second into the TFTR plasma, and the scattered radiation is synchronously detected. A previous version of the alpha particle scattering experiment for TFTR was to have used a 200 kW gyrotron with a scattering geometry that was substantially off perpendicular from the magnetic field in order to eliminate the lower hybrid effect on the scattered spectrum and measure the full alpha particle slowing down feature.

In the present experiment, whose main components are illustrated in Figure 1, the scattering geometry will be nearly perpendicular to the magnetic field to take advantage of the lower hybrid resonance. This resonance begins at approximately the ion plasma frequency for scattering nearly perpendicular to the magnetic field. In the simulated spectrum of Figure 2, this corresponds to a scattered frequency of approximately 60.38 GHz, or a fluctuation in the plasma at approximately 380 MHz. Equivalently, this frequency corresponds to an alpha particle energy of approximately 1 MeV, as shown in Figure 3. As the scattering radiation within the transmitted Gaussian beam becomes less perpendicular to the magnetic field, the lower hybrid resonance moves out to higher frequencies which corresponds to higher alpha particle energies. In Figure 3, the alpha particle birth energy of 3.5 MeV corresponds to a scattered frequency of approximately 60.72 GHz in Figure 2, which is a fluctuation at approximately 720 MHz within the plasma. This resonance will increase the scattering cross section by up to 3 orders of magnitude from the originally proposed experiment. The power requirement of the scattering source has been reduced by a like amount to obtain the same signal to noise performance. However, a minimum power of at least 0.1 kW is required to provide enough signal to noise performance to determine the thermal deuterium and tritium densities and velocity distributions which determine the lower frequency behavior of the scattered spectrum.

Detecting the thermal ion feature simultaneously with the higher frequency alpha particle signal will more precisely establish the alpha

particle density and velocity distribution function. An absolute calibration of the scattering system would normally be required to measure the thermal ion and alpha densities. However, a relative measurement of the alpha density to the thermal deuterium and tritium densities is easily accomplished without an absolute measurement. The TFTR interferometer will be used to calibrate the thermal ion density with a knowledge of Z_{eff} and ion impurity spatial distribution from the TFTR Z_{eff} diagnostics.

The main disadvantage of scattering perpendicular to the magnetic field is that the lower hybrid feature may be altered by inhomogeneous plasma effects and is possibly more sensitive to a particular alpha particle energy in which the phase velocity of the lower hybrid wave is close to the alpha particle velocity. Another disadvantage is that the lower hybrid resonance is sensitive to the value of the fluctuating wave vector, $k \approx |k_s - k_j|$, which is determined by ray tracing. Therefore, accurate ray tracing of the Gaussian beams through the plasma is imperative to reduce the error of the resulting data analyses.

The transmitted beam will be launched in the extraordinary mode (X-mode) at approximately half the electron cyclotron harmonic frequency. The background plasma emission, which is due primarily to relativistically down-shifted electron cyclotron emission, was 25 eV on TFTR shot 55851, which is a high performance supershot typical of that expected during D-T operation. The receiver antenna will also be arranged to detect X-mode.

Plasma refraction will slightly bend the transmitted and received beams when the plasma refractive index changes significantly from unity. This occurs if the plasma density increases to the point at which the 60 GHz wave would approach the X-mode cutoff for perpendicular propagation to the magnetic field. For TFTR, the X-mode wave will be able to propagate to the core of the plasma for densities below $1.5 \times 10^{14} \text{ cm}^{-3}$. Refraction will become noticeable at central densities greater than approximately $6-7 \times 10^{13} \text{ cm}^{-3}$.

The initial arrangement of the scattering diagnostic will have low loss waveguide for both the transmitter and receiver with scanning antennas which can be moved between shots. The existing scanning antennas are part of the TFTR microwave scattering diagnostic [18], which is a 60 or 70 GHz, 0.1 Watt scattering experiment that makes use of an extended interaction oscillator (EIO). Multiple plasma shots will be required to scan spatial profiles and explore possible anisotropies in the alpha particle velocity distribution.

This experiment will use three techniques to reduce the effects of stray gyrotron radiation into the receiver. First, the transmitted beam will be deposited on existing carbon tiles, which are angled to scatter

the radiation toroidally. This will reduce the amount of radiation in the poloidal plane of scattering. Second, the receiver will have notch filters, which could reject up to 60 dB of unshifted gyrotron radiation. Finally, the initial receiver will be a homodyne receiver, in which a small amount of the gyrotron power will be mixed with the received radiation. The unshifted gyrotron radiation will then be from DC to several tens of Hertz, depending on the final gyrotron intrinsic linewidth, and an intermediate frequency amplifier will be used to amplify a bandwidth from 5-1500 MHz. If the stray gyrotron radiation can be reduced by the two previous methods to less than 200 mW, which is the damage threshold of the RF mixer, then the detection electronics of the receiver will not be affected by stray light. This 5-1500 MHz bandwidth will then be mixed with a 9.44 GHz oscillator, to frequency up convert the received bandwidth into the filter bank's range of operation.

III. SIMULATED SCATTERED SPECTRUM

The calculated post-detection signal to noise ratio for a typical D-T plasma is shown in Figure 2. The post detection signal to noise calculation is $SNR_{PD} = [P_s / (P_s + P_n)] \times (BW \times t)^{1/2}$, where P_s is the predetection signal power, P_n is the predetection receiver and plasma background noise power, BW is the receiver channel bandwidth and t is the integration time. The predetection signal power is based on 1 kW gyrotron power, and the predetection noise power is assumed to be 25 eV. This calculation has spatially integrated the transmitter and receiver Gaussian beam patterns. Plasma refraction was not included in this calculation, and is presently being put into our computer codes. The result is expected to be similar, but the shape of the spectrum will be modified because the fluctuating wavenumber changes with refraction. A signal to noise ratio greater than 10 is desired for the data reduction to result in an error less than 5% for the alpha density, the alpha birth energy, and the slowing down distribution function critical velocity, or mean energy for a Maxwellian distribution function. For Figure 3, the highest signal to noise ratio corresponds to an alpha particle energy of approximately 1 MeV, and the signal to noise ratio is 10 or greater up to approximately 2 MeV. The spatial resolution will vary from 10 to 30 cm depending on the scattering geometry of the transmitter and receiver. For a 1 kW gyrotron, the temporal resolution for acceptable signal to noise ratios could be as small as 5 msec.

This diagnostic will also measure energetic ions produced during neutral beam and ICRF heated plasmas. In addition, thermal ions, such as the fuel D and T ions, will be measured automatically in the low frequency range of the scattered spectrum. Since the scattering will be

performed perpendicular to the magnetic field, the ion cyclotron harmonics should be observable for all ion species[19,20] with a 200 Megasample/sec digitizer. The ion species can then be determined by measurement of the observed ion cyclotron frequencies which are directly proportional to the ions' charge to mass ratio. This provides the advantage of determining the densities and velocity distribution functions of all ion species simultaneously. Therefore, the deuterium and tritium fuel mixture could be observed as their ion cyclotron harmonics change in intensity and linewidth with alpha particle production. Other ion impurities may also be determined by their ion cyclotron harmonics.

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

REFERENCES

1. Evans, D. E., and Katzenstein, J., *Rep. Prog. Phys.*, Vol. 32, (1969), 207-271.
2. Sheffield, J., *Plasma Scattering of Electromagnetic Radiation*, Academic Press, New York, 1975.
3. Bowles, K. L., *Phys. Rev. Let.*, Vol. 1, pp. 454-455, December 15, 1958, and also National Bureau of Standards, Boulder, CO, Report No. 6070, (1959).
4. Booker, H. G., *Journal of Geophysical Research*, Vol. 64, No. 12, pp. 2164-2177.
5. Daehler, M. and Ribe, F. L., *Physical Review*, Vol. 161, No. 1, pp. 117-125, September 5, 1967.
6. Evans, D. E., Forrest, M. J. and Katzenstein, J., *Nature*, No. 5057, pp. 21-23, October 1, 1966.
7. Kronast, B., Röhr, H., Glock, E., Zwicker, H. and Fünfer E., *Phys. Rev. Let.*, Vol. 16, No. 24, pp. 1082-1085, June 13, 1966.
8. Röhr, H., *Zeitschrift für Physik*, 209, pp. 295-310 (1968)
9. Daehler, M., Sawyer, G. A. and Thomas, K. S., *Physics of Fluids*, Vol. 12, No. 1, pp. 225-229 (January 1969)
10. Goehlich, A., Schulz-von der Gathen, V. and Dobeles, H. F., *Plasma Physics and Controlled Fusion*, Vol. 33, No. 1, pp. 29-40 (1991).
11. Behn, R., et. al., *Phys. Rev. Let.*, Vol. 62, (1989), pp. 2833-2836.
12. Hughes, T. P., and Smith, S. R. P., *J. Plasma Physics*, Vol. 42, Part 2, (1989), pp. 215-240.
13. Hughes, T. P., and Smith, S. R. P., *Nuclear Fusion*, Vol. 28, No. 8, (1988), pp. 1451-1457.
14. Chiu, S. C., *Physics of Fluids B*, Vol. 3, No. 6, (June 1991), pp. 1374-1380.
15. Aarnodt, R. E., and Russell, D. A., *Nuclear Fusion*, Vol. 32, No. 5, (1992), pp. 745-755.
16. Vahala, L., Vahala, G. and Sigmar, D. J., *Nuclear Fusion*, Vol. 26, No. 1, (1986), pp. 51-59.
17. Woskov, P. P., et. al., *Rev. Sci. Instrum.*, Vol. 59, No. 8, (August 1988), pp. 1565-1567.
18. Bretz, N., Efthimion, P., Doane, J., and A. Kritz, *Rev. Sci. Instrum.*, Vol. 59, No. 8., (August 1988), pp. 1538-1543.
19. Machuzak, J. S., et. al., *Rev. Sci. Instrum.*, Vol. 59, No. 8, (August 1988), pp. 1562-1564.
20. Machuzak, J. S., (1990) PhD thesis, Massachusetts Institute of Technology.

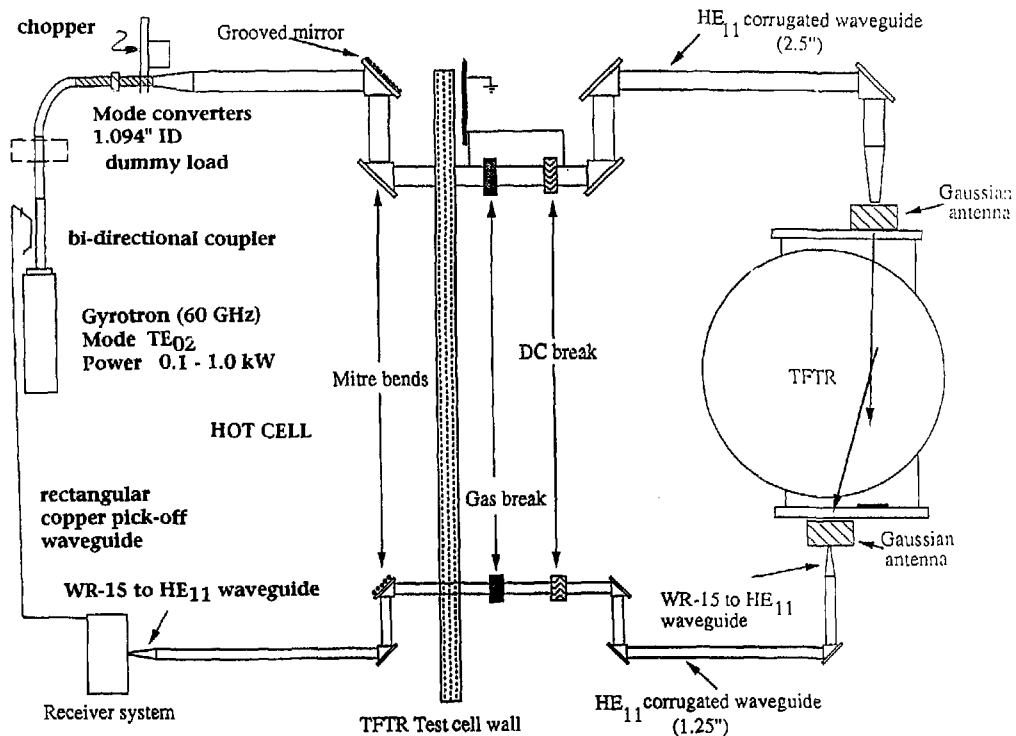


Figure 1. Schematic of the TFTR alpha particle scattering diagnostic.

TFTR Integrated Transmitter and Receiver Beam SNR Spectrum

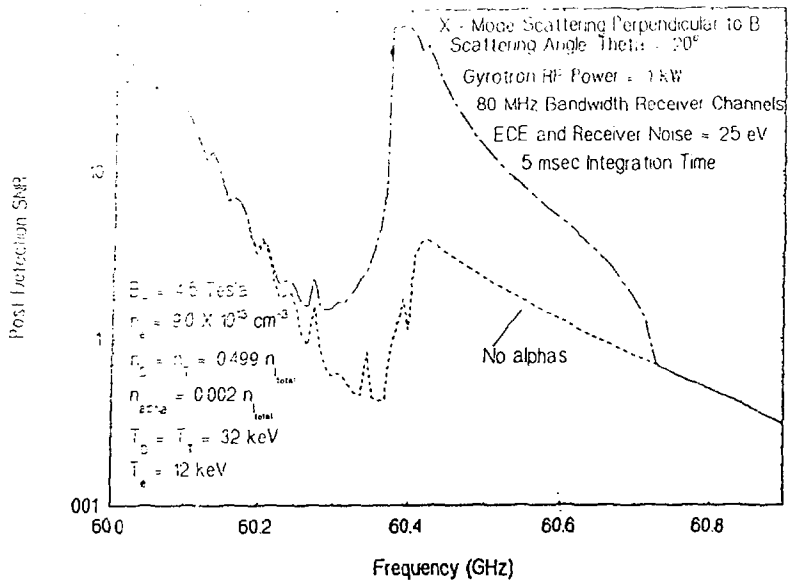


Figure 2. Simulated scattered spectrum for a D-T TFTR plasma shot.

TFTR Integrated Transmitter and Receiver Beam SNR Spectrum

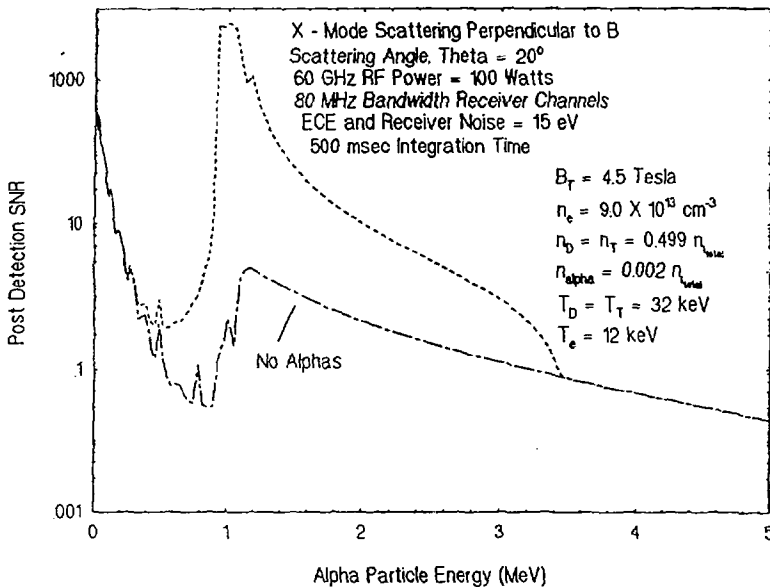


Figure 3. Simulated scattered spectrum for a D-T TFTR plasma shot as a function of alpha particle energy.