

Title: Progress Toward A Microsecond Duration, Repetitive, Intense-Ion Beam for Active Spectroscopic Measurements on ITER

RECEIVED

JUN 11 1996

OSTI

Author(s): Harold A. Davis, P-24 R. Richcard Bartsch, P-22
 Cris W. Barnes, P-24 Joseph C. Olson, Varian Ion Implant Sy
 William A. Reass, P-24 Henry M. Schlienitz, *
 Don M. Coates, * J. W. Hunt, *
 R. H. Loveberg, ** J. B. Greenly, ***
 * DuPont Central Research and Development
 ** University of California, San Diego, CA (emeritus)
 *** Cornell University, Laboratory of Plasma Studies, Ithaca, NY

Submitted to: 11th High Temp Plasma Diagnostic Conference
 Monterey, CA
 June 13-17, 1996
 Also to be published in Rev. of Scientific Instruments

MASTER



Los Alamos
 NATIONAL LABORATORY

Los Alamos National Laboratory, an affirmative action/equal opportunity employer, is operated by the University of California for the U.S. Department of Energy under contract W-7405-ENG-36. By acceptance of this article, the publisher recognizes that the U.S. Government retains a nonexclusive, royalty-free license to publish or reproduce the published form of this contribution, or to allow others to do so, for U.S. Government purposes. The Los Alamos National Laboratory requests that the publisher identify this article as work performed under the auspices of the U.S. Department of Energy.

DISTRIBUTION OF THIS DOCUMENT IS UNLIMITED *ng*

DISCLAIMER

Portions of this document may be illegible in electronic image products. Images are produced from the best available original document.

**Progress Toward a Microsecond Duration, Repetitive,
Intense-Ion Beam for Active Spectroscopic Measurements on ITER**

H.A. Davis, R. R. Bartsch, C.W. Barnes, J.C. Olson, W.A. Reass

Mail Stop E526, Los Alamos National Laboratory, Los Alamos New Mexico 87545

H. M. Scheinitz, D. M. Coates, J. W. Hunt

DuPont Central Research and Development, Wilmington, Delaware 19880

R. H. Lovberg^{***}

4744 Panorama Drive, San Diego CA 92116

and

J. B. Greenly

Cornell University, Laboratory of Plasma Studies, Ithaca, New York 14853

Abstract

We describe the design of an intense, pulsed, repetitive, neutral beam based on magnetically insulated diode technology for injection into ITER for spectroscopic measurements of thermalizing alpha particle and thermal helium density profiles, ion temperature, plasma rotation, and low Z impurity concentrations in the confinement region. The beam is being developed to enhance low signal-to-noise ratios expected with conventional steady-state ion beams because of severe beam attenuation and intense bremsstrahlung emission. A 5 GW (e.g., 100 keV, 50 kA) one-microsecond-duration beam would increase the signal by 10^3 compared to a conventional 5 MW beam with signal-to-noise ratios comparable to those from a chopped conventional beam in one second.

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

Introduction

Charge-exchange recombination spectroscopy^{1,2} (CXRS) is now the primary diagnostic of ion temperature, rotational velocity, and helium ash concentration³ in Tokamaks. Using visible spectroscopic views across a neutral beam which provides the charge exchange source for fully stripped ions in the plasma, CXRS provides good spatial localization of the Doppler-shifted and broadened light. Present Tokamaks are able to use the same neutral beams used for heating the bulk plasma for the CXRS source. The 100--120 keV energy of these positive-ion-source, neutral beams is well matched to the peak of the charge exchange cross-section. Future large, high-density Tokamaks such as ITER are faced with a serious problem. Positive-ion-source neutral beams will not penetrate the plasma and are not suitable for core heating. High-energy negative-ion-source beams planned for heating interact at too high an energy with the plasma ions and too low of a cross-section to produce useful CXRS signals.⁴ Steady-state beams provide a CXRS signal which increases linearly with plasma density, while the bremsstrahlung background increases quadratically. In high-density operation of ITER, it is expected that only in the outer half of the plasma can CXRS signals be seen by modulating the beam and phase averaging over a few seconds^{5,6}; ion temperature and helium ash density in the central core of the plasma would be unmeasurable.

¹ R. J. Fonck, D. S. Darrow and K. P. Jaehnig, Phys. Rev. A **29** 3288 (1984).

² R. J. Fonck, and R. A. Hulse, Phys. Rev. Lett. **52** 530 (1984).

³ E. J. Synakowski, R. E. Bell, R. V. Budny, C. E. Bush, P. C. Efthimion, B. Grek, D. W. Johnson, L. C. Johnson, B. Leblanc, H. Park, A. T. Ramsey, and G. Taylor, Phys. Rev. Lett. **75** 3689 (1995).

⁴ G. Schilling and E. J. Synakowski, Rev. Sci. Instrum. **63** 4937 (1992).

⁵ E.S. Marmor, in the *Proceedings of the International School of Plasma Physics "Piero Caldirola"*, Workshop on Diagnostics for ITER, Aug. 28 - Sept. 1, 1991 Varenna, Italy.

⁶ E. S. Marmor these proceedings.

It was proposed that intense ion diode technology could be adapted to make a diagnostic neutral beam source.⁷ Instead of steady (or slowly modulated) beams with less than 1 A/cm^2 beam density, microsecond pulses of a few kA/cm^2 (at the beam focus in the reactor) would be used. Operated at 100 keV/AMU near the peak of the CXRS cross-sections, these beams would increase signal-to-noise ratios because of their high intensity coupled with very short gating times on the detectors to reduce the bremsstrahlung background. Not only would these beams provide vital measurements in the plasma core, but would do so with time resolution governed by the repetition rate of the beam. Such a neutral beam was developed⁸ and it was demonstrated that effective charge neutralization could be achieved in a gas cell at current densities of 20 A/cm^2 (only at factor of 3-7 below the required value depending on the diode diameter), answering the primary scientific question of the approach.

Many of the remaining key issues in the application of intense ion-diode technology to diagnostic neutral beams have largely been solved, albeit not simultaneously: pulse lengths of longer than $1\text{ }\mu\text{s}$ have been achieved with careful attention to magnetic geometry; more than 90 % of the ion diode beam can be at full-energy; and active plasma anodes (see discussion below about plasma anodes) have achieved more than 90 % hydrogen for cleanliness⁹. Beam divergences less than 0.8° (FWHM) have been demonstrated.¹⁰ This is within a factor of two of the divergence needed to maintain the desired current densities in ITER over the required 15 m source-plasma distance required if the beam source is to be located outside the biological

⁷ D. J. Rej, I. Henins, R. J. Fonck and Y. J. Kim, Rev. Sci. Instrum. **63** 4934 (1992).

⁸ R. R. Bartsch, H. A. Davis, I. Henins and J. B. Greenly, Rev. Sci. Instrum. **66** 306 (1995).

⁹ W. A. Noonan, S. C. Glidden, J. B. Greenly and D. A. Hammer, Rev. Sci. Instrum. **66** 3448 (1995).

¹⁰ D. J. Johnson, R. J. Leeper, W. A. Stygar, R. S. Coats, T. A. Mehlhorn, J. P. Quintenz, S. A. Slutz and M. A. Sweeney, J. Appl. Phys. **58** 12 (1985).

radiation shielding wall with adequate room for valves and the neutralizing cell. The light-ion inertial confinement fusion program regularly proposes such divergences to make intense ion beam implosion schemes plausible, but some development may be required. The remaining technical issue is, demonstrating repetitive beam operation, is discussed in the remainder of the paper.

Over the past two decades researchers in United States, Germany, Russia, and Japan, have been investigating the application of intense-pulsed-ion beam technology ($E = 1\text{-}30\text{ MeV}$, $I = 0.1\text{ to }1\text{ MA}$, $\tau = 10\text{-}50\text{ ns}$)^{11,12} to inertial confinement fusion defense and energy programs. More recently (over the past decade), using more modest beam parameters ($E = 0.1\text{-}1.0\text{ MeV}$, $I = 0.005\text{-}0.05\text{ MA}$, $\tau = 100\text{-}1000\text{ ns}$), research into the processing of materials using this technology has emerged^{13,14,15}. Other applications such as high-flux neutron sources and neutral beam sources for Tokamak diagnostics, the subject of this paper, also appear promising.

These beams are produced in vacuum, magnetically insulated diodes requiring a source of ions, an accelerating voltage, and a magnetic field transverse to the acceleration gap to suppress electron flow and enhance the ion flow (fig. 1). Ion currents typically exceed the vacuum space-charge limit by 5-50 times owing to electrons confined in the acceleration region by the applied magnetic field. The beams are produced and transported in vacuum of at least 10^{-4}

¹¹ V. M. Bystriskii and A. Didenko, *High Power Ion Beams* (American Institute of Physics, New York, 1989).

¹² R. N. Sudan, in *Inertial Confinement Fusion*, edited by A. Caruso and E. Sindoni [International School of Plasma Physics "Piero Caldirola" (Varenna), Italian Physical Society, Bologna, 1989] p. 453.

¹³ H. A. Davis, G. E. Remnev, R. W. Stinnett, and K. Yatsui, *Mater. Res. Soc. Bull.*, Aug. 1996 (in Press).

¹⁴ K. Yatsui, X. D. Kang, T. Sonogawa, T. Matsuoka, K. Masugata, Y. Shimotori, et. al., *Phys. of Plasmas*, **1** 1730 (1994).

¹⁵ G. E. Remnev, and V. A. Shulov, *Lasers and Particle Beams* **11** 707 (1993).

Torr. Traditionally ions are drawn from the surface of a polymer anode¹⁶ converted to a plasma by a combination of high-voltage flashover and electron impact. Polymer anodes are unacceptable for applications requiring repetitive operation because of limited lifetime, excessive heat loading, and high gas production. Also polymer anodes produce excessive debris, have poor uniformity and reproducibility, and do not allow the selection of the ion species (typically these beams have a mix of hydrogen and carbon ions). Anodes, that draw ions from a pre-formed plasma are being developed at a number of laboratories to overcome the above limitations.^{9,17, 18} Some of these anodes allow the selection of any gaseous ion species including hydrogen isotopes and helium. Traditional single-shot beam accelerators (using Marx generators and high-voltage pulse lines), incompatible with repetitive operation are yielding to new high-average power beam accelerators. An ion beam system operating at 100 Hz (in 10-shot burst mode, since no active cooling was available)⁹ and a 300 keV intense beam source at 0.3 Hz¹⁹ have been demonstrated.

Diode Design

The first diode used on the Los Alamos CHAMP (Continuous High Average-Power Microsecond Pulser) accelerator will be for a variety of applications including materials processing studies and will use a magnetically insulated extraction diode^{20,21} with plasma anode in ballistically focused geometry (45° full focusing angle with 30-cm focal length). Extension to a straight unfocused beam or longer focal length beams for Tokamak diagnostics is straight

¹⁶ D. J. Rej, R. R. Bartsch, H. A. Davis, R. J. Faehl, J. B. Greenly, and W. J. Waganaar, *Rev. Sci. Instrum.* **64** 2753 (1993).

¹⁷ S. Humphries Jr., R. J. Anderson, J. R. Freeman, and J. Greenly, *Rev. Sci. Instrum.* **52** 162 (1981).

¹⁸ J. B. Greenly, M. Ueda, G. D. Rondeau, and D. A. Hammer, *J. Appl. Phys.*, **63** 1872 (1998).

¹⁹ I. F. Isakov, V. M. Matvienko, M. S. Opekunov, G. E. Remnev, and Y. P. Usov, *Vacuum* **42** 159 (1991).

²⁰ R. N. Sudan and R. V. Lovelace, *Phys. Rev. Lett.* **31** 1174 (1973).

²¹ M. P. Desjarlais, *Phys. Fluids B* **1** 1709 (1989).

forward requiring only different anode and cathode angles with respect to the system axis. The diode shown in fig. 1 operates as follows. The anode consists of a flat pulsed induction coil²² in an aluminum housing. The high-voltage coil is formed from four parallel sets of two turn spiral windings coaxial with the system axis. The coil in focusing geometry is dished in the form a cone having a normal to the surface of 22.5° with respect to the system axis. The plasma anode is formed by first radially ducting a puff of gas with a fast acting valve (risetime $\sim 100 \mu\text{s}$), located on axis, over the coil surface. The valve will be actuated by a metallic diaphragm driven either by eddy currents or a voice-coil mechanism. When the gas puff is properly distributed, a fast rising current pulse ($10 - 20 \text{ kA}$, $\tau_{\text{rise}} = 1-2 \mu\text{s}$), delivered to the induction, coil breaks the gas down and induces azimuthal current in the plasma at the coil surface. The $j_\theta \times B_r$ force on the plasma accelerates the plasma to the radial opening in the aluminum anode housing where it is stagnated against the applied radial magnetic field and where ions can be extracted. Higher frequency oscillations at 8 MHz will be induced in the windings to promote rapid and complete ionization of the gas. The cathode consists of the tips of two thin concentric metal conical sections (or cylinders for unfocused geometry). The gap between the cathode tips and the plasma anode is 2 cm. Just before application of the accelerating voltage, a $200 \mu\text{s}$ risetime magnetic field of about 1.5 kG is applied transverse to the anode-cathode gap by two magnetic field coils -- one located inside the inner cone and one located outside the outer cone. At peak field and when the plasma is in position at the anode housing aperture, a positive accelerating voltage supplied from a high-voltage modulator is applied to the anode. The applied magnetic field strength is adjusted to prevent electrons from crossing the anode-cathode gap, but the more massive ions, only very

²² C. L. Dailey and R. H. Lovberg, AIAA paper 79-2093, Oct. 1979.

weakly deflected by the magnetic field, have approximately linear trajectories. The insulating transverse magnetic field ($B \sim 2 B_{\text{crit}}$, where B_{crit} is the minimum field for insulation of the electrons given by the condition that the electron gyro-radius equals the anode-cathode gap for electrons with kinetic energy given by the voltage drop across the diode) will be generated by two magnetic field coils on the grounded cathode focusing cones. The expected beam parameters are $E = 200 - 250 \text{ keV}$, $I = 15 \text{ kA}$, and $t = 1 \text{ } \mu\text{s}$ or about 3.4 GW nearly equal to the 5 GW proposed diagnostic system.

We have modeled the dynamics of the plasma layer, using a snowplow type model which assumes the plasma is entrained by a thin, conducting current sheet driven away from the coil surface by currents in the inductive coil. The plasma was modeled in planar geometry. The model solves the coupled circuit equation and the equation of motion of the plasma with a model for the plasma resistivity derived from previous experimental data.²³ The circuit inductance as a function of current sheet position from the coil surface required for these calculations is determined from calculations of the magnetic field for various current sheet positions (fig. 2) to be given by the expression:

$$L(z) = L_0 (e^{-z/z_0}), \text{ where } z_0 = 1.35 \text{ cm}, z = \text{the current sheet position above the coil surface, and } L_0 = 993 \text{ nH} .$$

The procedure used was to vary the capacitor charge voltage so that the plasma is brought to rest against the applied magnetic field at the diode gap entrance. For a gas fill of 2.5×10^{15} molecules/cm³ corresponding to 80 mTorr of D_2 at the coil surface before acceleration (this density was chosen to insure good gas breakdown), a capacitor charge voltage of 14 kV is required. The

²³ R. H. Lovberg and C. L. Dailey, NASA Contract Report No. 191155, 1994.

stored electrical energy is 50 J. It takes 1.5 μ s for the plasma to be driven into position at the anode housing aperture with a peak current sheet velocity of just over 20 km/s (fig. 3).

Finite element thermal modeling of the coil at 30 Hz has been performed since the electrically insulating material surrounding the high-voltage windings is a poor thermal conductor preventing removal of heat dissipated in the windings by thermal conduction. It was found that without a supplemental means to transfer heat dissipated in the coil, unacceptably high temperatures on the order of 600^o C develop in the coil. Three solutions to this problem were investigated: (1) increase the thermal conductivity of the epoxy insulator by filling it with high-thermal-conductivity material such as diamond dust; (2) transfer the heat from the windings to the aluminum coil housing with heat pipes; and (3) remove the heat by flowing a cooling medium such as air, water or oil through hollow windings. The model results indicated that all three methods would reduce the maximum temperature of the coil, but that the flowing coolant was the most effective.

Electrical Design

A key system parameter, the pulse duration, was chosen from a study of overall system electrical efficiency including plasma formation and magnetic-field energy requirements, scaling of diode performance from the Los Alamos Anaconda accelerator operated with 1 μ s pulses, Tokamak diagnostic signal-to-noise optimization, thermal transport modeling of beam energy deposition in targets (for materials applications), and electrical engineering considerations. The beam electrical system requires many modulator sub-systems synchronized with each other and the ion acceleration pulse (fig. 4). A gas puff modulator and the induction coil modulator sub-system will be housed in a "hotdeck" chassis at common potential with the pulsed anode.,

For electrical insulation, fiber optic cables will carry fast control and diagnostic signals.

Solid-state switches will be used to deliver current from storage capacitors to the magnetic field coils at ground potential. Energy recovery techniques will be used in the final design, although in initial tests energy recovery will be omitted for simplicity. A dedicated fast sequence and monitor system will confirm the proper sub-system parameters before the main acceleration pulse is initiated to minimize damage to components in case of off-normal operation.

The accelerating power system will utilize 4 parallel type "E" Blumlein lines each switched with a English Electric Valve CX1736AX thyatron. This tube is a 11.4-cm diam., 70 kV, two gap, hollow anode device. The hollow anode design was selected because it permits reverse voltage and current up to 50% of the maximum rating in the event of diode mis-match. We selected Blumlein lines rather than convention pulse lines because they provides an output pulse voltage into a matched load equal to the charge voltage rather than half the charge voltage. This reduces by two the transformer turns ratio, and the number of parallel thyatrons required. The lower turns ratio decreases the transformer leakage inductance enabling pulse rise and fall times to be decreased by a factor of four. A benefit of the "E" type Blumlein line choice is the end inductors nearest the transformer and thyatrons can be trimmed to offset the transformer leakage and thyatron inductances. The number of networks comprising each Blumlein line will depend on the beam energy spread required by each application. For materials applications, square voltage and current waveforms are not desired since a spread in ion energy leads to a more uniform deposition profile in targets (this eliminates the Brag peak near the end of the ion range produced by a monoenergetic beam). For diagnostic applications, monoenergetic beams are preferred to optimize charge exchange and to simplify data interpretation. Figure 4 shows a

calculation of the voltage pulse shape for an seven element (on each side of the load) Blumlein line.

The accelerator will be housed in a metal tank approximately 2 m x 2m x 2 m. The overall system length including the vacuum system, but not the neutralizer is about 3 m. The initial system will use recycled capacitors for the Blumlein lines to minimize development cost. With higher energy density state-of-the-art capacitors the modulator footprint could be reduced significantly. The modulator tank will be filled with high-voltage transformer oil having a density of about one. The system shown is configured for materials processing. For a diagnostic beam the sample chamber would be absent giving an overall system length of about 3.5 - 4.0 m. An estimates of the electrical efficiency is $30 \pm 10\%$ including power to make the plasma and the pulsed magnetic field. Thus for a 5 GW peak power system, at 30 Hz the time averaged power consumption will be in the neighborhood of 500 kW.

Sponsored by Los Alamos, Laboratory Directed Research and Development under US DOE contract W-7405-ENG-36).


electronic mail: davis@lanl.gov

** current address: Varian Ion Implant Systems, 508 Dory Road, Glouchster, MA 01930-2297

***University of California, San Diego, CA (emeritus)

Figures

1. Active plasma anode diode layout.
2. Magnetic flux surfaces for the inductive coil with the plasma current sheet located at two distances from the coil surface: a) 0.5 cm and b) 3.0 cm.
3. Position (z) and velocity (v) versus time of the plasma layer for a D_2 fill density of 2.5×10^{15} cm^{-3} and capacitor charge voltage of 14 kV. The circuit current time history I is also shown.
4. Block diagram of the electrical circuits.
5. Accelerating voltage waveform for a 7 element Blumlein line with transform coupling coefficient of 0.98 with a 15 Ohm resistive load.

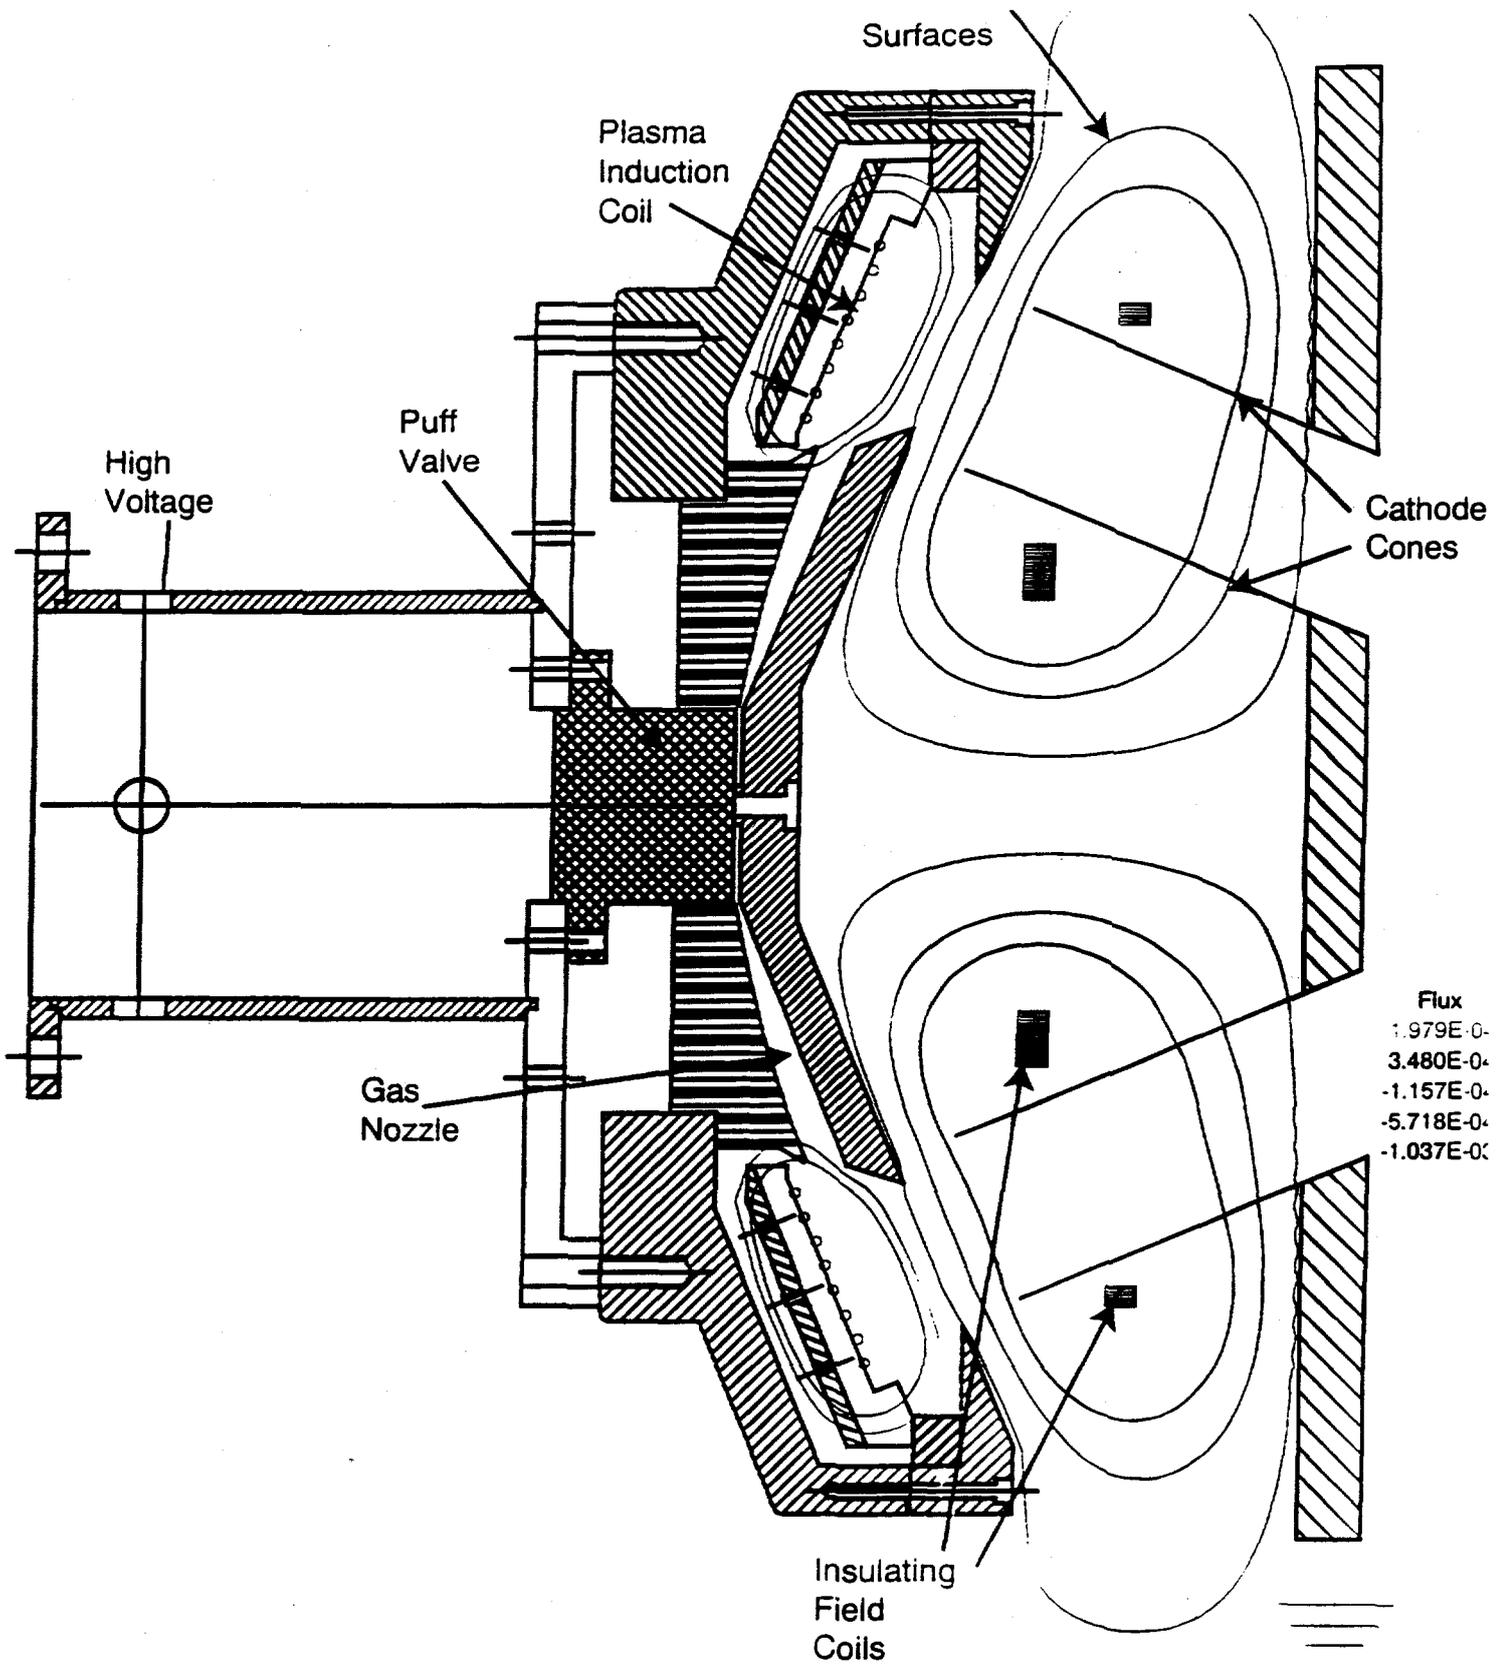



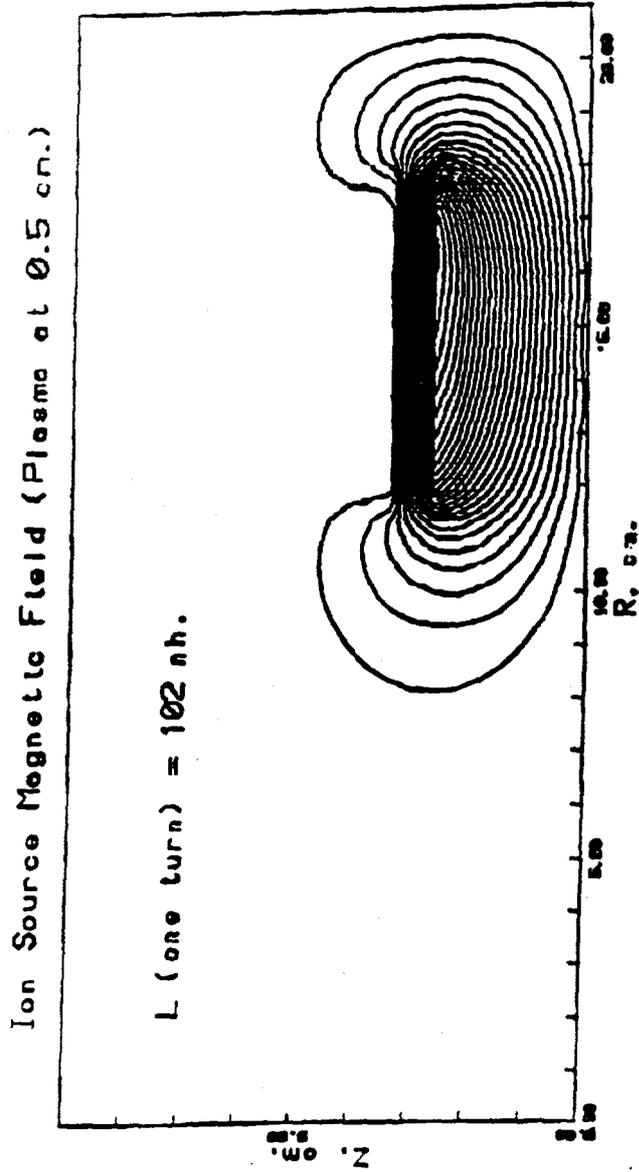


Figure 2 a


Ion Source Magnetic Field (Plasma at 3 cm.)

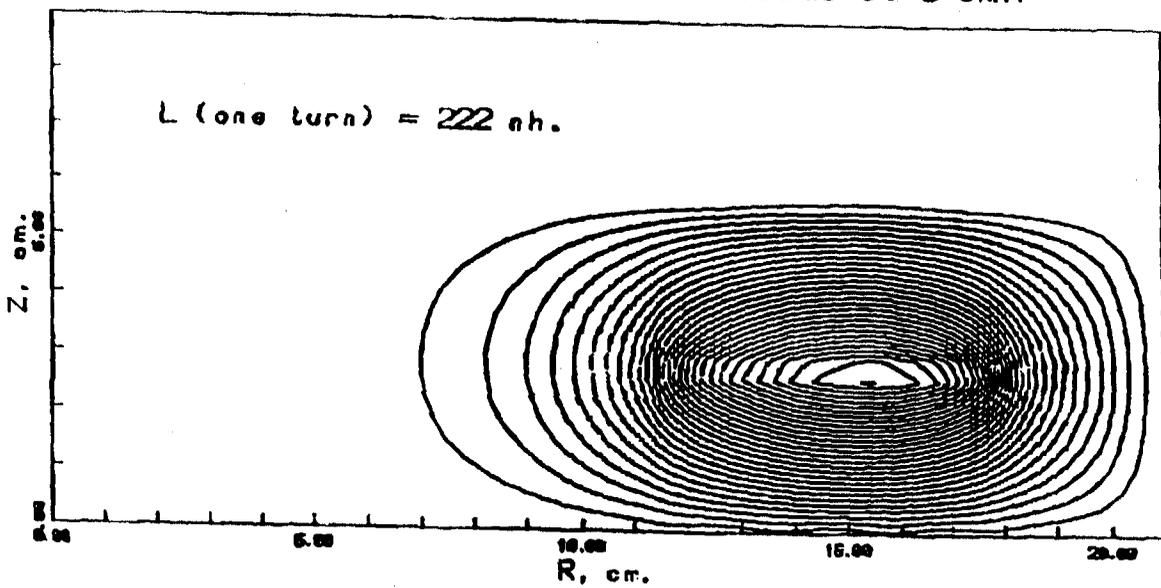

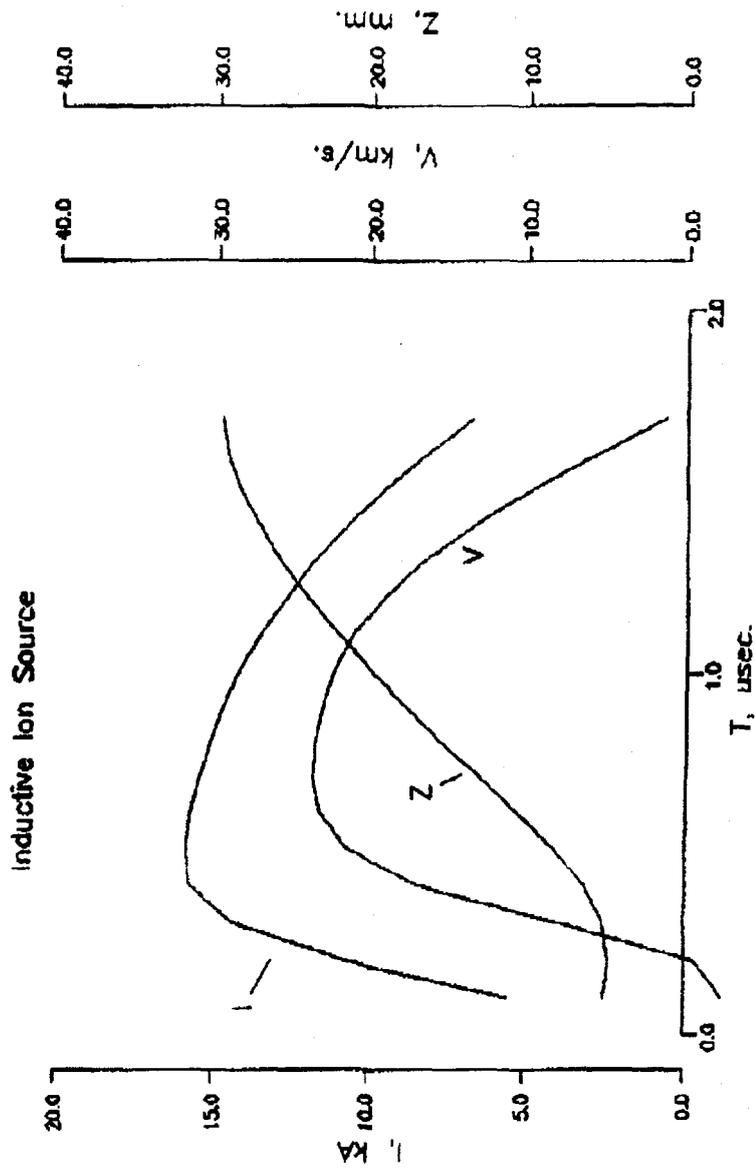

$M = 0.02 \text{ mg}$
 $V = 14 \text{ kV}$
 $(\approx 15 \text{ cm}^{-3} D_2)$

Fig 3

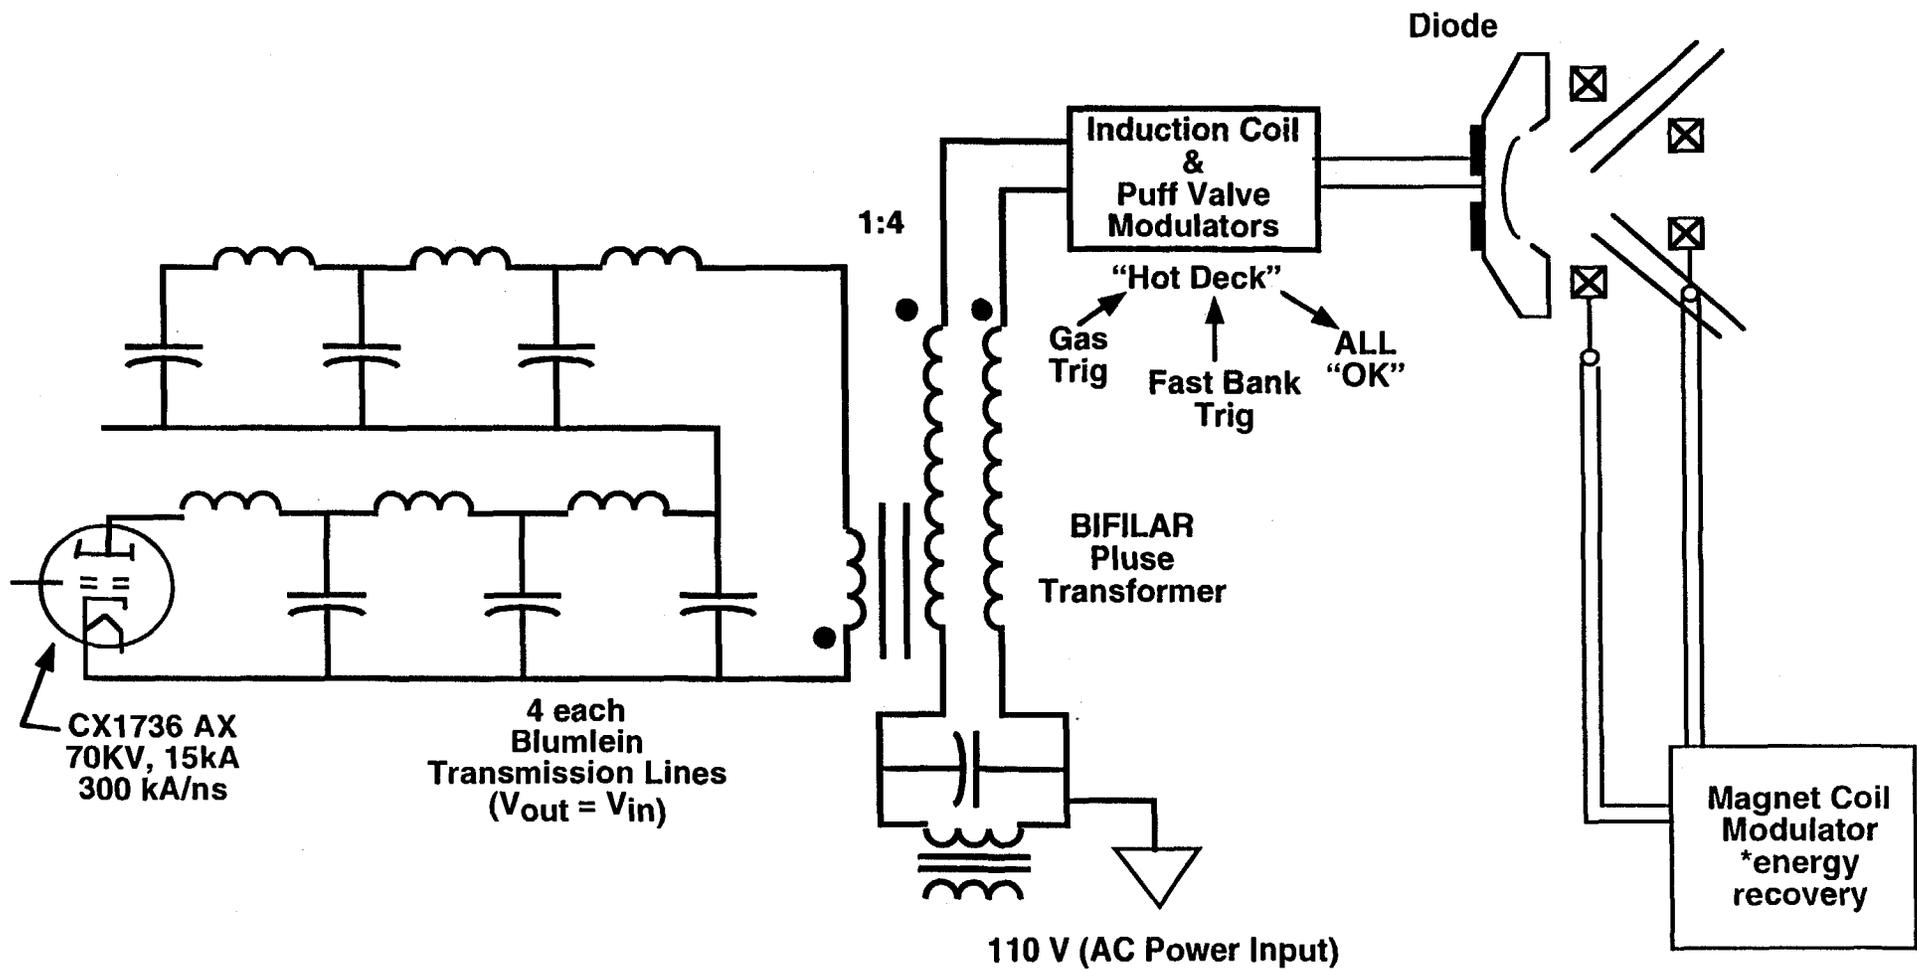

15 " true length = 38.1 cm reduce to 21 %

