

# ***EPR Dosimetry - Present and Future***

**D.F. Regulla**

*GSF - National Research Centre for Environment and Health,  
Institute of Radiation Protection,  
85764 Neuherberg,  
Germany*



**MX0000319**

## **Abstract**

*In the past, IAEA has played a central role in stipulating research and development in EPR high-dose standardisation as well as in coordinating and organising international dose intercomparison programs, within the Member States of the United Nations from the mid-seventies till today. The future tasks of EPR dosimetry seem to tend towards different subjects such as biomarkers, biological radiation effects, post-accident dose reconstruction in the environment, and retrospective human dosimetry. The latter may be considered a promising tool for epidemiology on the way to re-define radiation risk of man for chronicle radiation exposures, based on e.g. South Ural civil population and radiation workers. There are on-going international activities in the field of standardising high-level dosimetry by the American Standards on Testing and Materials (ASTM), and by the International Organisation of Standards (ISO). The International Commission on Radiation Units and Measurements (ICRU) is considering the establishment of relevant recommendations concerning industrial radiation processing, but also human dose reconstruction*

## **1. Introduction**

High-level application of ionising radiation from 10<sup>3</sup> to 10<sup>6</sup> Gy was described in the early seven-ties. The growing field of industrial radiation processing, under the aspects of safety and economy, was soon recognised to require a reliable and accurate dosimetry<sup>(1)</sup>. There were dosimetry techniques available at that time, but traceability to primary standards, access to national calibration services or availability of international recommendations on standardisation of high dose dosimetry were limited.

It was in 1977 that the Agency took initiative and invited international experts to discuss new methods of dosimetry and standardisation in radiation processing at the occasion of a Consultants' Meeting on High-Dose Standardisation and Intercomparison for Industrial Radiation Processing<sup>(2)</sup>. Decision was taken to accept a proposal of the author and implement

a "new" technique based on radiation induced generation of radicals in an amino acid, i.e. alanine<sup>(3)</sup>. Electron paramagnetic resonance (EPR) spectrometry was chosen for quantification of the radical concentration. Within the subsequent IAEA co-ordinated research programme, EPR became a scientific tool for dosimetric application in routine and metrology<sup>(4,5)</sup>. Later, the Agency established the International Dose Assurance Service (IDAS) to the member states of IAEA using the meanwhile standardised alanine/EPR technique. IDAS was operated jointly between IAEA and GSF<sup>(6)</sup>. Since 1991 the Agency continues to offer IDAS successfully as an exclusive service supplier<sup>(7,8)</sup>.

The forthcoming manuscript will not deal with archaeological and geological dating<sup>(9,10)</sup> nor with EPR imaging<sup>(11)</sup>. It should however be noted that it is particularly the task of geological dating for human sciences that stipulated great interest and initial progress in EPR dosimetry<sup>(12)</sup>.

## 2. Present Status

### 2.1. The alanine/EPR system

Alanine/EPR dosimetry uses organic crystalline amino acids (e.g. alanine,  $\text{CH}_3\text{-CHNH}_2\text{-COOH}$ ) as a sample material<sup>(3)</sup>. The dosimetry method is applicable to dosimetry of different types of radiation as well as, within limits, to dosimetry in mixed radiation fields, e.g. x and gamma rays, beta radiation, accelerator electrons, protons<sup>(13)</sup>, neutrons<sup>(14)</sup>, and ions<sup>(15-18)</sup>.

**Table I**  
**Chemical, Physical and Dosimetric Properties of the GSF Alanine/EPR Dosimetry System**

Composition	Alanine $\text{CH}_3\text{-CHNH}_2\text{-COOH}$ (85 %) and paraffin (15 o/o)
Effective atomic number	$Z_{\text{eff}} \approx 7.2$ (tissue: $Z_{\text{eff}} \approx 7.4$ )
Specific gravity	$\approx 15 \text{ g/cm}^3$
Dimensions	4.9 mm in diameter x 10 mm length
Measuring quantity, $D_w$	Absorbed dose to water; otherwise on request
Measuring range	$0.5 \text{ Gy} < D_w < 5 \cdot 10^5 \text{ Gy}$
Detection threshold	0.05 Gy
Dose rate dependence	Not detectable till to 1011 Gy.h <sup>-1</sup>
Energy dependence	Approx. independent, for $E_{\text{ph}} \geq 100 \text{ keV}$ and $E_e \geq 1 \text{ MeV}$
Irradiation temperature $\theta$	Negligible or correctable in the range $-90^\circ\text{C} < \theta < +70^\circ\text{C}$ ( $k_\theta = 0.0018 \text{ }^\circ\text{C}^{-1}$ for $D \leq 40 \text{ kGy}$ )
Fading (signal loss) within 2 years	$< 1\%$ at $22^\circ\text{C}$ and $< 70\%$ r.h.
Interspecimen scattering	1 s.d. $\leq \pm 0.5\%$ , within a batch
Interbatch scattering	$\leq 1\%$
Precision	$u \leq \pm 1.5\%$ at 95 % confidence level, approved by national laboratory intercomparison protocol, at $> 10 \text{ Gy}$
Electron/photon ratio of response	1.0, for $E_e > 1 \text{ MeV}$
Neutron/photon ratio of response	about 0.6, for $E_n > 0.1 \text{ MeV}$

The free radicals in crystalline biomolecules are relatively stable interim products in a chain of events, that similar to tissue start with the absorption of radiation energy. Since free radicals take key positions in the chain of events which lead to biological damage in cell structures, the quantification of free radicals in alanine can even be used for a biologically relevant dosimetry.

Accurate EPR dosimetry provides the availability of an appropriate "system" as well as qualified personnel with know-how, experience and care. The essential system components are: Alanine detectors of a high purity production and metrological quality, a high performance EPR spectrometer and an air-conditioned laboratory, calibration facilities in the respective dose range, as well as dosimeters of secondary standard or reference quality level, whose calibration is traceable to the primary standards of national laboratories (Fricke dosimetry, calorimetry, ionisation chamber dosimetry). Essential dosimetric properties, as evaluated at GSF, are compiled in the Table I.

## ***2.2. Radiation processing: Reference and transfer dosimetry***

Meanwhile a number of acknowledged national laboratories world-wide started to use the alanine/EPR technique for quality control programs in radiation processing. The alanine/EPR technique has been introduced for quality control also in therapy<sup>(19)</sup> using the alanine/EPR technique similar to the IDAS programme<sup>(21,22)</sup>. Future applications will probably be based on a new EU Medical Devices Directive<sup>(20)</sup>.

## ***2.3. Therapy-level dosimetry***

The properties of alanine/EPR dosimetry have always been studied with an eye focussing on radiation therapy<sup>(23)</sup>. The advantages of alanine/EPR dosimetry in this field are evident, e.g. the dynamic dose range, the archival character of dose information based on a non destructive readout that allows for repeated EPR measurements and sample storage, and the tissue equivalency of detector samples. The latter property makes the method applicable also in high-energy radiation dosimetry without the impact of perturbation and displacement effects as known from ionisation chamber dosimetry. A mathematical method based on Fast Fourier Transform has meanwhile been developed capable to filter background and simultaneously noise in the frequency domain of EPR spectra<sup>(24)</sup>; it provides significantly higher resolved alanine/EPR signals, and this down to about 50 mGy.

It is again the Agency which at an early stage has organised an alanine/EPR intercomparison in the therapy-level range<sup>(25)</sup> and has recently established a Co-ordinated Research Project aimed to implement alanine/EPR dosimetry into an IDAS-type quality assurance service in future<sup>(26)</sup>. Complementary investigations are reported on the use of alanine EPR dosimetry in proton therapy<sup>(27,28)</sup>.

## ***2.4. Identification of irradiated food***

For a long period of time there has been a lack of appropriate identification methods of irradiated foodstuffs which situation has changed during the past decade<sup>(29)</sup>. A variety of methods has become available to evaluate on the status of radiation processing, or even roughly estimate the dose level, valid for irradiated spices and spice products, herbs, dried vegetables, some kind of fruits, coffee beans, different meats and meat products as well as fish, shell-fish, shrimps, etc.<sup>(30)</sup>. EPR spectroscopy has turned out applicable to the identifi-

cation of irradiated foods, for discrimination against unirradiated foods or exclusion of two- or more-fold food irradiations<sup>(31-36)</sup>. Some food allows an EPR dose assessment within  $\leq 5\%$ <sup>(37)</sup>. For a relevant Food Control Dosimetry Network based on EPR, standard EPR spectra from the above foods should be available to be transferred for calibration and measurement, between laboratories and authorities involved by internet.

### **2.5. Ultra high-level dosimetry**

Since material fatigue of radiation sensitive components is an imported factor in nuclear fuel safety, it should carefully be checked before the components are implemented in the facility construction, and be under continued control during operation. Dose control by an appropriate dosimetry technique is inevitable for this task. For quantification of doses up to 108 Gy and above, EPR spectroscopy based on crystalline detectors was developed for irradiation temperatures of up to several hundred degrees Celsius<sup>(38,39)</sup> and verified by Monte Carlo based simulation of the radiation transport<sup>(40)</sup>.

### **2.6. Standards and recommendations**

Principles, procedures and quantities used in the alanine/EPR technology are described in an ASTM standard<sup>(41)</sup> which is on the way to be implemented in an ISO standard<sup>(42)</sup>. ICRU considers to establish a task group on "Dosimetry in Industrial Uses of Ionising Radiation"<sup>(43,44)</sup>. An ICRU recommendation in this field would be of great interest and need, for public acceptance, benefit and health as far as dosimetry is concerned for radiation preserved food, sterilised pharmaceuticals, and medical and health care products<sup>(29)</sup>. IAEA and other international and national bodies, e.g. WHO, FAO, CEC and FDA, should be invited to contribute to the recommendation with their great expertise and the available technical documents.

### **2.7. EPR spectrometry**

Alanine/EPR dosimetry uses sophisticated research EPR spectrometers in the X band microwaves. The state of the art of this equipment, in course of time, and its future potential are described by Ettinger<sup>(45)</sup>, Pilbrow<sup>(46)</sup> and Ikeya<sup>(47)</sup>. Routine dosimetry makes use of meanwhile available table-top EPR spectrometers with permanent magnets. Interesting parametric improvement of equipment as well as procedures has recently been proposed<sup>(48,49)</sup>. A pitch-activated alanine detector type<sup>(50)</sup> or the use of an in-cavity  $Mn^{++}$  standard<sup>(51)</sup> offer approaches to introduce individual calibration factors for alanine samples. The use of a constant rotation goniometer reduces the effect of response anisotropy and results into reduced detection limits<sup>(52)</sup>. Large-scale alanine dosimetry services in national or international quality control may profit from automatic sample changing devices by robot<sup>(53)</sup> or magazine type mechanisms<sup>(54)</sup>. Future in situ oriented biophysical dosimetry will make use of EPR spectroscopy applying different microwave bands and magnetic field strengths<sup>(55,56)</sup>.

## **3. Future Tasks**

EPR spectroscopy has started playing a role in tooth dosimetry in the late seventies addressed to victims of Hiroshima and Nagasaki. Since scientists started in the nineties to work on dose histories of individuals from the early nuclear production plants of the former

Soviet Union, remarkable progress has been achieved in extending the lower detection limit of this material.

### **3.1. Biophysical dosimetry**

So far, the most known biological dosimetry technique is based on chromosome analysis in peripheral human Lymphocytes serving in cases of acute exposures, dose estimates above 100 mGy, and a number of victims for evaluation<sup>(57)</sup>. Further improvement is expected from the so-called fluorescence in situ hybridisation (FISH) method based on translocations<sup>(58,59)</sup>.

The to-day the biophysical EPR dosimetry using tooth (and bone) samples from exposed victims may represent a potential completion of the biological dosimetry for reasons of accuracy, reliability, dose individuality and procedural simplification<sup>(60,61)</sup>. EPR dosimetry is based on radiation induced radicals in hydroxyapatite, which is the mineral phase of teeth and bones. The most stable radical known is CO<sub>2</sub><sup>(62)</sup>, which life time has been reported to 107 years (at 25°C)<sup>(63)</sup>. At present doses from about 50 mGy to above 100 Gy can be evaluated, which range complies with potential accidental doses<sup>(64,65)</sup>, including photon and electron radiation as well as potentially  $\alpha$ -particles and ions<sup>(66)</sup>.

### **3.2. Environmental dose reconstruction and accident dosimetry**

Management of dose assessment from objects of man's environment can profit from the free radical generation in and EPR spectroscopy of many deserted objects<sup>(67)</sup>, e.g. sugar<sup>(68)</sup>, pharmaceuticals<sup>(69)</sup>, egg shells<sup>(70,71)</sup>, cellulose<sup>(72)</sup> and pot-scale<sup>(73)</sup>. In future, also the mineral phase of soil and bricks<sup>(74,75)</sup>, building materials<sup>(76)</sup> and appropriate tissues of animals<sup>(77)</sup> will be considered more intensively. Subsequently, accidental doses of individuals can be derived from material doses of the human environment by computational conversion if not directly assessed from teeth and bone samples<sup>(78-80)</sup>. Cases of evaluating doses, by EPR, from radioactive sources or radioactive scrap metal in public areas or in possess of private persons became known in the recent past<sup>(81)</sup>.

### **3.3. Retrospective dosimetry**

Biophysical EPR dosimetry is on the way to become a tool of increasing interest for retrospective dosimetry, i.e. evaluation of individual exposures that occurred years or decades and more ago<sup>(82)</sup>. It was first described by Ikeya et al. for the atomic bomb survivors of Hiroshima and Nagasaki<sup>(83)</sup>, later for victims of the Chernobyl accident<sup>(84,85)</sup>, nuclear workers of the PO Mayak<sup>(64)</sup>, and residents of the Techa river valley, the latter both in the Southern Ural region<sup>(86)</sup>. A valuable survey is given in (87). ICRU has meanwhile established a working group in the field of retrospective dosimetry, the IAEA a co-ordinated research project in the same field.

### **3.4. Uncertainties in retrospective dosimetry**

Individual and environmental retrospective dosimetry may serve, e.g. for verification of dose records as a basis for epidemiological studies. Comparisons with risk data from Hiroshima and Nagasaki require careful consideration of uncertainties. The uncertainties cover, e.g., the EPR spectrometer, sampling, sample treatment and evaluation procedures, the impact of influence parameters (e.g. ultraviolet light, diagnostic x-rays; etc.), calibration,

and the statistical treatment of data<sup>(88,89)</sup>. Future research tasks in this domain should focus unbiased scientific attention to identify component uncertainties and evaluate overall uncertainties<sup>(90-93)</sup>.

## **4. Perspectives**

### **4.1. Emergency network for dosimetry**

The capability of EPR to contribute to emergency response dosimetry was recently under consideration<sup>(94)</sup> demonstrating a rapid analysis method for screening deciduous teeth of children in the days and weeks following a radiation accident<sup>(95)</sup>. Such a response could conceivably aid in medical and social decision making.

Also of importance are the savings of time and manpower and the increase in reliability which could be achieved in dose reconstruction if identification and collection of biological and environmental dosimetry materials were promptly undertaken. The complexity of reconstructing doses from a population year after an accident would be greatly reduced if consideration were given to the task immediately following an accident<sup>(96)</sup>. Protocols for such response are currently not available<sup>(97)</sup>.

### **4.2. Basis for juridical consequences**

EPR based dose reconstruction will compete and equally complement the established biological dosimetry in the future, particularly in accidental or emergency dosimetry cases. Contrary to biological methods, the biophysical methods will allow to evaluate doses reliably for all those exposures of humans which occurred decades and more ago. The achievements to be expected represent new perspectives for labour inspection authorities in cases of radiation accidents at work and for the juridical consequences in cases of prosecution or legitimate claims for compensation.

### **4.3. Epidemiology and redefinition of radiation risk**

Interest in the new perspectives of EPR dosimetry will hold particularly also for retrospective dosimetry of individuals with long-term exposures where the traditional biological methods may be of limited use only, e.g. for the determination of exposures of radiation workers from nuclear centres starting in the forties. Individual retrospective dosimetry based on tooth tissues and bones, also for the verification of corresponding film dosimetry records, may help us together with available health records of those radiation workers, to redefine radiation risk for - contrary to the acute exposure in Hiroshima and Nagasaki - chronic exposure of man. First evaluations showed a reduced risk for leukaemia<sup>(98)</sup>.

### **4.4. Biomedical dosimetry: The human as an *in vivo* dosimeter and space biodosimetry**

On the horizon we may, in not a too far future, discover new techniques of EPR or magnetic resonance (MR) spectrometry for human *in vivo* dose evaluation<sup>(99)</sup> and local dose imaging after accidents, e.g. *non invasive* dosimetry from teeth, skeleton, cell membranes and other tissues capable to produce and store radiolysis products detectable with EPR spectrometry. This might probably lead to a presently still visionary development of a "whole body dose scanner", equivalent to the established whole body counter. The human body appears to

represent a still widely undiscovered field for dosimetry - and an exciting reservoir for radiation research also in future<sup>(100)</sup>.

Such dosimetry techniques lead to the further vision of an individual biodosimetry, e.g. for space missions, providing dosimetry that can not be lost, inappropriately handled or manipulated by an individual, and a permanent record of cumulative doses due to different radiation types<sup>(101,102)</sup>.

## 5. Concluding remarks

Present dosimetry techniques in radiation processing, also EPR, will in future be supplemented by new, e.g. radiofluorescence type, techniques for routine and quality control programmes<sup>(103,104)</sup>. For treatment planning of products the experimental dosimetry may be supplemented by dose computations based on source-target modelling. The necessary product parameters for absorption and scatter can be transferred from a central data bank, by the world wide web<sup>(105)</sup>. Its implementation shows new perspectives to exchange information between processing plants, trade companies, and authorities, and will make the radiation processing level of a product traceable. The internet can equally serve to check the local dosimetry quality of a processing plant by a future telemetrology, whose technique and logistics has still to be developed and established<sup>(106)</sup>. The internet will facilitate the exchange of dosimetry results, calibration and traceability certificates as well as of acceptance passports for products - to be verified by EPR dosimetry.

By contrast, the importance of EPR for biophysical dosimetry promises to expand in future. Unification and standardisation will allow individual dose reconstruction in emergency cases which tool was not available earlier<sup>(81, 107-115)</sup>. Apart from the mineral tooth enamel, it is the metabolic dentine which can probably provide additional EPR information on e.g. bone seekers. Also this potential will continue to keep scientific interest focussed on EPR biophysical dosimetry in future<sup>(116,117)</sup>.

The present duties of the world-wide SSDL network for radiation protection radiation application in medicine, could in principle be considered a basis for expansion to biophysical - accident and retro-spective - dosimetry and a first step towards a concept of a world-wide operating "Integrated Retro-spective Dosimetry Network"<sup>(94,118)</sup>. It could provide permanent assistance and expertise in bio-physical dosimetry, probably in co-operation with other national or regional laboratories, that can offer biological dosimetry, whole body counting and bioassays, as well as thermally and optically stimulated luminescence dosimetry techniques for objects taken from an incidental environment (Figure 1).

A future integrating tool in the Integrated Retrospective Dosimetry Network could be the generation and use of purposely created age, sex and size specific voxel phantoms that should be considered for the evaluation of organ, tissue and risk relevant dose quantities due to external exposure<sup>(119)</sup>, and particularly internal exposures from incorporated radionuclides<sup>(120)</sup>. The dose computations may use existing conversion coefficients or be performed by numerical dosimetry using Monte Carlo codes<sup>(119,121)</sup>. For individual doses closer to the actual exposure and risk they may require local ethnical voxel phantoms for reference, e.g. for the Techa river population and Mayak workers. For the future benefit of victims, for fast decisions as a basis of medical treatment, and for qualified information of authorities and the public, the above strategies appear worth being considered now.

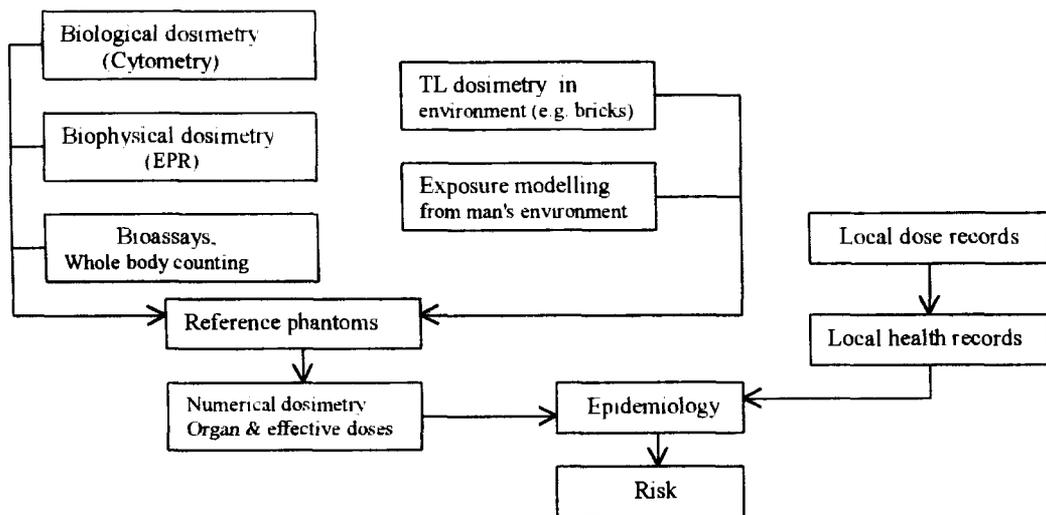


Figure. 1. Schematic model for tasks and objective of an Integrated Retrospective Dosimetry Network, for further discussion(94,118).

## 6. References

Part of the references refer to manuscripts presented at the recent "International Conference on Biodosimetry and 5th International Symposium on ESR Dosimetry and Applications", Obninsk/Moscow, Russia, 22-26 June 1998"; they are under process of peer-reviewing, and planned to be published in the International Journal of Applied Radiation and Isot. in 1999. Extended abstracts are available from the Conference Book of Abstracts (Prof. A. Tsyb, or Dr. Y. Skoropad, Medical Radio-logical Research Center of Russian Academy of Medical Sciences, Obninsk, email address: (mrrc@obninsk.ru). A condensed review on the development and achievements of EPR dosimetry and applications in the post two decades can be found in: "ESR Dosimetry and Applications", *Appl. Radiat. Isot.* 40 (1989) 829-1246; 44 (1993) 1-468; and 47 (1996) 1151-1687, as well as in: "Retrospective Dosimetry - Physical and Biological Aspects", *Radiat. Prot. Dosim.* 77 (1998) 1-138.

- (1) WORLD HEALTH ORGANIZATION. *Wholesomeness of Irradiated Food, Report on a Joint FAO/IAEA/WHO Expert Committee 1980. WHO Technical Reports Series 659, Geneva (1981).*
- (2) *High-dose Standardization and Intercomparison for Industrial Radiation Processing, Report of a Consultants' Meeting, IAEA, Vienna (1977).*
- (3) REGULLA, D.F., DEFFNER, U., *Dosimetry by EPR spectroscopy of alanine. Appl. Radiat. Isot.* 33 (1982) 1101-1114.
- (4) SCHARMANN, A., *ESR - A scientific tool for applications. Appl. Radiat. Isot.* 40 (1989) 829-834.
- (5) McLAUGHLIN, W.L., *Radiation processing dosimetry - past, present and future. these Proceedings.*

- (6) NAM, W.J., REGULLA, D.F., *The significance of the International Dose Assurance Service for radiation processing. Appl. Radiat. Isot.* 40 (1989) 953-956
- (7) METHA, K., "Report of the Second Research Co-ordination Meeting (RCM) for the Co-ordinated Research Project (CRP E2 40 06) on Characterisation and Evaluation of High-dose Dosimetry Techniques for Quality Assurance in Radiation Processing", *SSDL Newsletter No. 39, IAEA, Vienna (1998) 19-31.*
- (8) METHA, K., *High-dose dosimetry programme of the Agency. these Proceedings.*
- (9) GRUN, R., *Present status of ESR-dating. Appl. Radiat. Isot.* 40 (1989) 1045- 1055.
- (10) SKINNER, A., *The maturing of a technique. Is ESR still an "experimental" technique? Appl. Radiat. Isot. (in press, 1999).*
- (11) EATON, G.R., EATON, S.S., MALTEMPO, M.M., *Three approaches to spectral-spatial EPR imaging. Appl. Radiat. Isot.* 40 (1989) 1227-1231.
- (12) IKEYA, M. (Ed.), *EPR Dating and Dosimetry*", Ionics Publications Co. Ltd., Japan (1985) 1-538.
- (13) ONORI, S., D'ERRICO, F., DE ANGELIS, C., EGGER, E., FATTIBENE, P., JANOVSKY, I., *Proton response of alanine based pellets and films. Appl. Radiat. Isot.* 47 (1996) 1201-1204.
- (14) SCHRAUBE, H., WEITZMEGGER, A., WIESER, A., REGULLA, D.F., *Fast neutron response of alanine probes. Appl. Radiat. Isot.* 40 (1989) 941-944.
- (15) HUTTERMANN, J., SCHAEFER, A., *Heavy-ion-induced free radical formation in solid DNA-constituents: Quantitative and structural aspects. Appl. Radiat. Isot.* 40 (1989) 915-921.
- (16) WALIGORSKI, M.P.R., DANIALY, G., KIM SUN LOH, KATZ, R., *The response of the alanine detector after charged-particle and neutron irradiation. Appl. Radiat. Isot.* 40 (1989) 923-933
- (17) HITOSHI KOIZUMI, TSUNEKI ICHIKAWA, HIROSHI YOSHIDA, *Radiation chemistry in alanine irradiated with g-rays and ion beams. Appl. Radiat. Isot.* 47 (1996) 1205-1210.
- (18) CESELSKI, B., STUGLIK, Z., WELOPOLSKI, L., ZVARA, I., *The effect of high LET radiation on the dynamics of microwave power saturation of EPR signal in alanine. Appl. Radiat. Isot. (in press, 1999).*
- (19) BARTOLOTTA, A., INDOVINA, F.L., ONORI, S., ROSATI, A., *Dosimetry for cobalt-60 gamma rays with alanine. Radiat. Prot. Dosim.* 9 (1984) 277-281.
- (20) GAO JUNCHENG, *The NIM alanine-ESR dosimetric system for industrial radiation processing. Appl. Radiat. Isot.* 47 (1996) 1161-1164.
- (21) REGULLA, D.F., BARTOLOTTA, A., DEFFNER, U., ONORI, S., PANTOLONI, M., WIESER, A., *Calibration network based on alanine/EPR dosimetry. Appl. Radiat. Isot.* 44 (1993) 23-31.
- (22) COUNCIL DIRECTIVE ON MEDICAL DEVICES, 93/42/EEC, *Official Journal of the European Communities No. L 169, 14 June 1993.*
- (23) CHU, S., WIESER, A., FEIST, H., REGULLA, D.F., *EPR., Alanine dosimetry of high-energy electrons in radiotherapy. Appl. Radiat. Isot.* 40 (1989) 993-996.
- (24) RUCKERBAUER, F., SPRUNCK, M., REGULLA, D.F., *Numerical signal treatment for optimised alanine/EPR dosimetry in the therapy-level dose range. Appl. Radiat. Isot.* 47 (1996) 1263-1268.
- (25) NETTE, P., ONORI, S., FATTIBENE, P., REGULLA, D.F., WIESER, A., *Co-ordinated research efforts for establishing an international radiotherapy dose intercomparison service based on the alanine/EPR system. Appl. Radiat. Isot.* 44 (1993) 7-11.
- (26) METHA, K., GIRZIKOVSKY, R., *Alanine/ESR dosimetry for radiotherapy IAEA experience. Appl. Radiat. Isot.* 47 (1996) 1189-1192.

- (27) GALL, K., DESROSIERS, M., BENSEN, D., SERAGO, C., *Alanine EPR dosimeter response in proton therapy beams*. *Appl. Radiat. Isot.* 47 (1996) 1197-1200.
- (28) ROMANYUKHA, A.A., WIESER, A., REGULLA, D., *EPR dosimetry with different biological and synthetic carbonated materials*. *Radiat. Prot. Dosim.* 65 (1996) 389-392.
- (29) BOGL, K.W., REGULLA, D.F., SUESS, M.J. (Eds.), "Health Impact, Identification and Dosimetry of Irradiated Foods". WHO, Regional Office for Europe in co-operation with BGA-Federal Health Office, Neuherberg, Germany and GSF-National Research Centre for Environment and Health, Neuherberg, Germany. Report BGA/ISH 125. ISBN 3-89254-050-0 (1988) 155-161.
- (30) BOGL, K.W., *Identification of irradiated foods - Methods, development and concepts*. *Appl. Radiat. Isot.* 40 (1989) 1203-1210.
- (31) DODD, N.J.F., SWALLOW, A.J., LEY, F.J., *Use of ESR to identify irradiated food*. *Radiat. Phys. Chem.* 26 (1985) 451-453.
- (32) DODD, N.J.F., LEA, J.S., SWALLOW, A.J., *ESR detection of irradiated food*. *Nature* 334 (1988) 387.
- (33) RAFFI, J. EVANS, J.C., AGNEL, J.-P., ROWLANDS, C.C., LESGARDS, C., *ESR analysis of irradiated frogs' legs and fishes*. *Appl. Radiat. Isot.* 40 (1989) 1215-1218.
- (34) YORDANOV, N., GANCHEVA, V., *Studies on the possibilities for extension of the period for identification of irradiated herbs by the method of EPR*. *Appl. Radiat. Isot.* (in press, 1999).
- (35) DE JESUS, E., ROSSI, A., LOPES, R., *Identification and dose determination using ESR measurements in the flesh of irradiated vegetal products*. *Appl. Radiat. Isot.* (in press, 1999).
- (36) DESROSIERS, M.F., *Current status of the EPR method to detect irradiated food*. *Appl. Radiat. Isot.* 47 (1996) 1621-1628.
- (37) REGULLA, D.F., GOKSU, Y.H., VOGENAUER, A., WIESER A., *Retrospective dosimetry based on egg shells*. *Appl. Radiat. Isot.* 45 (1994) 371-373.
- (38) WESER, A., REGULLA, D.F., *EPR dosimetry in the giga-rad range*. *Appl. Radiat. Isot.* 40, 911-914 (1989)
- (39) ROTHFUCHS, T., DE LAS CUEVAS, C., DONKER, H., FEDDERSEN, H.-K., GARCIA-CELMA, A., GES, H., GOREYCHI, M., GRAEFE, V., HEJDRA, J., HENTE, B., JOCKWER, N., LEMEL, R., MONIG, J., MULLER, K., PRIJ, J., REGULLA, D., SMAILOS, E., STAUPENDAHL, G., TILL, E., ZANKL, M., "The HAW-Project: Test Disposal of Highly Radioactive Radiation Sources in the Asse Salt Mine", Final Rep. GSF 6/95, GSF, Neuherberg (1995) 1-238.
- (40) TILL, E., ZANKL, M., ROTHFUCHS, T., REGULLA, D., *Calculation of the radiation transport in rock salt using Monte Carlo methods*. *Nucl. Instrum. Meth. B* 111, 95-103 (1996).
- (41) AMERICAN STANDARDS FOR TECHNIQUES AND MATERIALS, *Standard practice for use of the alanine/EPR dosimetry system*. ASTM Standard E10.01-F (1994).
- (42) INTERNATIONAL ORGANISATION OF STANDARDS, ISO/TC85/WG3, AFNOR Paris and ISO, Geneva.
- (43) NEY, W.R., *The 1997 meeting of the ICRU*. *ICRU News Letters* 2 (1997) 14-15
- (44) NEY, W.R., *Plans for the 1998 meeting of the ICRU*. *ICRU News Letters* 1 (1998) 17.
- (45) ETTINGER, K.V., NAM, J.W., McLAUGHLIN, W.L., CHADWICK, K.H., "Progress in high-dose dosimetry". *Biomedical Dosimetry - Physical Aspects, Instrumentation, Calibration*, IAEA, Vienna (1981) 405-432.
- (46) PILBROW, J.R., *ESR fundamentals*. *Appl. Radiat. Isot.* 47 (1996) 1465-1470.
- (47) IKEYA, M., *New applications of electron spin resonance - Dating, Dosimetry and Microscopy*. World Scientific Publishing Co. Pte. Ltd., Singapore (1993).

- (48) BUGAY, A., KOLESNIK, S., Gaponenko, H., Alanine EPR dosimetry of therapeutic irradiators, these Proceedings.
- (49) BUGAY, A., KOLESNIK, S., TESLENKO, V., METHA, K., NAGY, V., DESROSIERS, M., Temperature stabilisation of alanine dosimeters used for food processing and sterilization. *Appl. Radiat. Isot.* (in press, 1999)
- (50) YORDONOV, N., New generation of self calibrated SS/EPR dosimeters - Alanine/EPR dosimeters, these Proceedings.
- (51) HASKELL, E.H., HAYES, R.B., KENNER, G.H., A high sensitive EPR technique for alanine dosimetry. *Radiat. Prot. Dosim.* 77 (1998) 43-49.
- (52) HASKELL, E.H., HAYES, R.B., KENNER, G.H., Improved accuracy of EPR dosimetry using a constant rotation goniometer. *Radiation Measurement* 27 (1997) 325-329.
- (53) SOLLER, T.J.L., MOSSE, D.C., CHARTIER M.M.T., JOLI, J.E., The LMRI ESR/alanine dosimetry system: Description and performance. *Appl. Radiat. Isot.* 40 (1989) 961-965.
- (54) SHARPE, P., SEPHTON, J., An automated system for measurement of alanine/EPR dosimeters. *Appl. Radiat. Isot.* (in press, 1999).
- (55) MAILER, D., SCHMALBEIN, D., A dedicated EPR analyser for dosimetry. *Appl. Radiat. Isot.* 44 (1993) 345-350
- (56) HOLE, E., SAGSTUEN, E., HAUGEDAL, S., NELSON, W., The nature of the major alanine and ENDOR studies of solid L-alanine X-irradiated at 295 K. *Appl. Radiat. Isot.* (in press, 1999).
- (57) BAUCHINGER, M., SCHMID, E., BRASELMANN, H., WILLICH, N., CLEMM, CH., Time-effect relationship of chromosome aberrations in peripheral lymphocytes after radiation therapy for seminoma. *Mutation Research* 211 (1989) 265-272.
- (58) SCHMID E., ZITZELSBERGER H., BRASELMANN H., GRAY J.W., BAUCHINGER M., Radiation-induced chromosome aberrations analysed by fluorescence in situ hybridisation with a triple combination of composite whole chromosome-specific DNA probes. *Radiat. Biol.* 62 (1992) 673-678.
- (59) LLOYD, D.C., New development in chromosomal analysis for biological dosimetry. *Radiat. Prot. Dosim.* 77 (1998) 33-36.
- (60) WIESER, A., GOKSU-OGELMAN, H.Y., REGULLA, D.F., VOGENAUER, A., Dose rate assessment in tooth enamel. *Quat. Sci. Rev.* 7 (1988) 491-495.
- (61) DESROSIERS, M.F., EPR bone dosimetry: a new approach to spectral deconvolution problems. *Appl. Radiat. Isot.* 44 (1993) 81-83.
- (62) CALLENS, F.J., VERBEECK, R.M.H., MATTHYS, P.F.A., MARTENS, L.C., BOESMAN, E.R., The contribution of CO33- and CO32- to the EPR spectrum near  $g = 2$  of powdered human tooth enamel. *Calcif. Tissue Int.* 41 (1987) 124-129.
- (63) SCHWARCZ, H.P., EPR study of tooth enamel. *Nucl. Tracks* 10 (1985) 865-867.
- (64) ROMANYUKHA, A. A., REGULLA, D., VASILENKO, E., WIESER, A., South Ural nuclear workers: Comparison of individual doses from retrospective EPR dosimetry and operational personal monitoring. *Appl. Radiat. Isot.* 45 (1994) 1195-1199.
- (65) ROMANYUKHA, A.A., DEGTEVA, M.O., WIESER, A., SEREZHENKOV, V.A., KOZHEUROV, V.P., VOROBIOVA, M.I., VASILENKO, E.K., KLESHCHENKO, E.D., IGNATEV, E.A., KOSHITA, A.A., SHISHKINA, E.A., KHOKHRYAKOV, V.F., Pilot study of the Ural region with EPR tooth dosimetry. *Proc. International Workshop on Chronic Exposure. Risk of Long-term Effects. Chelyabinsk (1995)*

- (66) STULIK, Z., MICHALIK, J., STACHOWICZ, W., OSTROWSKI, K., ZVARA, I., DZIEDZIC - GOCLAWSKA A., Bone powder exposed to the action of  $^{12}\text{C}$  and  $^{25}\text{Mg}$  ion beams as investigated by electron paramagnetic resonance spectroscopy. *Appl. Radiat. Isot.* 45 (1994) 1181-1187.
- (67) HASKELL, E.H., *Retrospective Accident Dosimetry using Environmental Materials.* *Radiat. Prot. Dosim.* 47 (1993) 297-303.
- (68) NAKAJIMA, T., Sugar as an emergency population dosimeter for radiation accidents. *Health Phys.* 55 (1988) 951-955.
- (69) REGULLA D.F., DEFFNER U., Dose estimation by EPR spectroscopy at a fatal radiation accident. *Appl. Radiat. Isot.* 40 (1989) 1039-1044
- (70) ODUWOLE A.D., SALES K.D. AND DENNISON K.J., Some EPR observations on bone, tooth enamel and egg shell. *Appl. Radiat. Isot.* 44 (1993) 261-266.
- (71) REGULLA, D.F., GOKSU, Y.H., VOGENAUER, A., WIESER A., Retrospective dosimetry based on egg shells. *Appl. Radiat. Isot.* 45 (1994) 371-373.
- (72) WIESER A., REGULLA D.F., "Cellulose for high-level dosimetry", *High Dose Dosimetry for Radiation Processing*, IAEA, Vienna (1991) 203-212.
- (73) WIESER A., GOKSU H.Y., REGULLA D.F. AND VOGENAUER A., Limits of retrospective accident dosimetry by EPR and TL with natural materials. *Radiat. Meas.* 23 (1994) 509-514.
- (74) PIVOVAROV, S., SEREDAVINA, T., RUIKHIN, A., ESR of environmental objects at Semipalatinsk Nuclear Test Site. *Appl. Radiat. Isot.* (in press, 1999).
- (75) OKA, T., IKEYA, M., ESR dosimetry using quartz grains in bricks. *Appl. Radiat. Isot.* (in press, 1999).
- (76) GINSBOURG, S.F., BABUSHKINA, T.A., BASOVA, L.B., KLIMOVA, T.P., ESR spectroscopy of building materials as a dosimetry technique. *Appl. Radiat. Isot.* 77 (1996) 1381-1383.
- (77) NASIROV, R., MOULUKOV, R., The g-irradiation dose measurement for animals of West Kazakhstan. *Appl. Radiat. Isot.* (in press, 1999).
- (78) SKVORTZOV, V., IVANNIKOV, A., WIESER, A., BOUGAI, A., BRIK, A., CHUMAK, V., STEPANENKO, V., RADCHUK, V., REPIN, V., KIRILOV, V., Retrospective individual dosimetry using EPR of tooth enamel. *The Radiological Consequences of the Chernobyl Accident*, EUR 16544 (KARAOGLOU, A., DESMET, G., KELLY, G.N., MENZEL, H.G. Eds.), Brussels (1996) 949-955.
- (79) WIESER, A., CHUMAK, V., BAILIFF, I., BARAN, N., BOUGAI, A., BRIK, A., DUBROVSKY, S., FININ, V., HASKELL, E., HAYES, R., IVANNIKOV, A., KENNER, G., KIRILLOV, V., KOLESNIK, S., LIIDJA, G., LIPPMAN, E., MAKSIMENKO, V., MATYASH, M., MEIJER, A., MINENKO, V., PASALSKAYA, L., PAST, J., PAVLENKO, J., PUSKAR, J., RADCHUK, V., SCHERBINA, O., SHOLOM, S., SKVORTSOV, V., STEPANENKO, V., VAHER, U., "International intercomparison of dose measurements using EPR spectrometry of tooth enamel", *The radiological consequences of the Chernobyl accident*, EUR 16544 (KARAOGLOU, A., DESMET, G., KELLY, G.N., MENZEL, H.G., Eds.), Brussels (1996) 957-964.
- (80) WU, K., GUO, L., CONG, J.B., SUN, C.P., HU, J.M., ZHOU, Z.S., WANG, S., ZHANG, Y., ZHANG, X., SHI, Y.M., Researches and applications of ESR dosimetry for radiation accident dose assessment. *Radiat. Prot. Dosim.* 77 (1998) 65-67.
- (81) HUTT, G., BRODSKI, L., POLYAKOV, V., Gamma-dose assessment after radiation accident in Kiisa (Estonia): Preliminary results. *Appl. Radiat. Isot.* 47 (1996) 1329-1334.
- (82) GRIFFITH, K.V., Retrospective dosimetry needs from an IAEA perspective. *Radiat. Prot. Dosim.* 77 (1998) 3-9.

- (83) IKEYA, M., MIYAJIMA, J., OKAJIMA, S., *EPR Dosimetry for atomic bomb survivors using shell buttons and tooth enamel*. *Jap J. Appl. Phys.* 23 (1984) L697-L699.
- (84) ISHII, H., IKEYA, M., OKANO, M., *EPR dosimetry of teeth of residents close to Chernobyl reactor accident*. *Nucl. Sci. Technol.* 27 (1990) 1153-1155.
- (85) SEREZFENKOV, V.A., DOMRACHEVA, E.V., KLEVEZAL, G.A., KULIKOV, S.M., KUZNETSOV, S.A., MORDVINCEV, P.I., SUKHOVSKAYA, L.I., SCHKLOVSKY-KORDI, VANIN, A.F., VOEVODSKAYA, N.V., VOROBEV, A.I., *Radiation dosimetry for residents of the Chernobyl region: A comparison of cytogenetic and electron spin resonance methods*. *Radiat. Prot. Dosim.* 42 (1992) 33-36.
- (86) WESER, A., ROMANYUKA A.A., KOZFEUROV, V.P., DEGTEVA, M.O., *Retrospective EPR dosimetry with teeth of Techa river residents, Intern. Workshop on the Scientific Bases for Decision Making after a Radioactive Contamination of an Urban Environment, Rio de Janeiro and Goiania, Bra-zil, 29 August - 2 September (1994)*
- (87) ROMANM)K ^ . A.A., IGNATEV, E.A., DEGTEVA, M.O., KOZFEUROV, V.P., WESER, A., JACOB, P., *Radiation doses from Ural region*. *Nature* 381 (1996) 199-200.
- (88) NAQY, V., *Accuracy problems in EPR dosimetry*. *Appl. Radial. Isot.* (in press, 1999).
- (89) HAYES, R.B., HASKELL, E.H., KENNER, G.H., *A mathematical approach to optimal selection of dose values in the additive dose method of EPR dosimetry*. *Radial. Meas.* 27 (1997) 315-323.
- (90) SKVORTSOV, V.G., IVANNIKOV, A.I., EICHHOFF, U., *Assessment of individually accumulated irradiation doses using EPR spectroscopy of tooth enamel*. *Molec. Struct.* 347 (1995) 321-329.
- (91) TERMINE, J.D., EANES, E.D., GREENFELD, D.J., VYLAN, M.U., HARPER, R.A., *Hydrazine-deproteinated bone mineral*. *Calcif. Tissue Res.* 12 (1972) 73-90.
- (92) IGNATEV, E.A., ROMANYUKHA, A.A., KOSHTA, A.A., WIESER, A., *A selective saturation method for EPR dosimetry with tooth enamel*. *Appl. Radiat. Isot.* 47 (1996) 333-337.
- (93) HASKELL, E., KENNER, G., HAYES, R., SHOLOM, S., CHUMAK, V., *An EPR intercomparison using teeth irradiated prior to crushing*. *Radiat. Meas* 27 (1997) 419-424.
- (94) REGULLA, D.F., *An integrated approach to retrospective dosimetry*. *IAEA Research Co-ordinated Meeting on the Use of Natural Materials for Solid State Dosimetry in Accident Zones and the Environment, Salt Lake City, Utah, USA, 25-29 January 1993.*
- (95) HASKELL, E.H., HAYES, R.B., KENNER, G.H., *An EPR dosimetry method for rapid scanning of deciduous teeth following a radiation accident*. *Health Phys.* (in press, 1999).
- (96) OLIVEIRA, A.R., VALVERDE, N.J.L., BRANDAO-MELLO, C.E., ALMEIDA, C.E.V., *Revisiting the Goiania accident: Medical and dosimetric experiences*. *Radiat. Prot. Dosim.* 77 (1998) 107-111
- (97) DESROSIERS, M., ROMANY-HA, A.A., "Technical aspects of the electron paramagnetic resonance method for tooth enamel dosimetry". *Biomarkers - Medical and Workplace Applications (MENDELSONH. M.L., MOHR, L.C., PEETERS, J.P. Eds.), Joseph Henty Press, Washington. D.C. (1998) 53-64.*
- (98) KOSHURNIKOVA, N.A., BULDAKOV, L.A., BYSOGOLOV, G.D., BOLOTNIKOVA, M.G., KOMILEVA, V.S., PETERNIKOVA, V.S., *Mortality from malignancies of the hematopoietic and lymphatic tissues among personnel of the first nuclear plant in USSR*. *Sc. Tot. Environm.* 142 (1994) 19-23.
- (99) MADER, K., GALLESZ, B., SWARTZ, H.M., *In vivo EPR: An effective new tool for studying patho-physiology, physiology and pharmacology*. *Appl. Radiat. Isot.* 47 (1996) 1663-1667.
- (100) SWARTZ, H.M., *In vivo EPR Proceedings of the 22nd International EPR Symposium, Denver, August 1-5, 1999 (in conjunction with 41st Annual Rocky Mountain Conference)*

- (101) HASKELL, E.H., HAYES, R.B., KENNER G.H., SHOLOM, S.V., CHUMAK, V.I., *Electron paramagnetic resonance techniques and space biodosimetry*, *Radiat. Res.* 148 (1997) S51-S59
- (102) IKEYA, M., *From earth to space: ESR dosimetry moves towards the 21st century*, *Appl. Radiat. Isot.* 44 (1993) 1-5.
- (103) REGULLA, D., *Lithium fluoride dosimetry based on radiophotoluminescence*, *Health Phys.* 22 (1972) 491-496.
- (104) KOVÁCS, A., BARANYAL, M., WOJNAROVITS L., SLEZSAK, J., McLAUGHLIN, W.L., MILLER S.D., MILLER, A., *A polymeric dosimeter film based on optically-stimulated luminescence for dose measurements below 1 kGy*, these Proceedings.
- (105) STENGER, V., HALMAVÁNSZKI, J., FALVI, L., FEHÉR I., DEMIREZEN, U., *Dose planning, read-ing and controls using PC at gamma radiation processes*, these Proceedings.
- (106) DESROSIERS M., *National Institute of Standards and Technology, Gaithersburg, M.D.*, personal communication, 1998.
- (107) SAGSTUEN, E., THEISEN, H., HENRIKSEN, T., *Dosimetry by ESR spectroscopy following a radiation accident*, *Health Phys.* 45 (1983) 961-968.
- (108) INI –INTERNATIONAL ATOMIC ENERGY AGENCY, *The Radiological Accident in Goiania*, IAEA, Vienna, STVPUB/815 (1988).
- (109) INTERNATIONAL ATOMIC ENERGY AGENCY, *The Radiological Accident in San Salvador*, IAEA, Vienna, STVPUB/847 (1990).
- (110) INTERNATIONAL ATOMIC ENERGY AGENCY, *The Radiological Accident in Soreq*, IAEA, Vienna, STVPUB/925 (1993).
- (111) CHUMAK, V., LIKHTAREV, S., SHOLOM, S., MECKBACH, R., KRJUCHKOV, V., *Chernobyl experience in field of retrospective dosimetry: Reconstruction of doses to the population and liquidators involved in the accident*, *Radiat. Prot. Dosim.* 77 (1998) 91-95.
- (112) IVANNIKOV, A., SKORTSOV, V., STEPANENKO, V., TSYB, A., *Tooth enamel EPR dosimetry: Progress and limitation*, *Appl. Radiat. Isot.* (in press, 1999).
- (113) ROMANYUKHA, A.A., REGULLA, D., VASLENKE, E.K., WIESER A., DROZHKO, E.G., LYZLOV, A.F., KOSHURNIKOVA, N.A., SHILNIKOVA, N.S., PANFILOV, A.P., *Verification of occupational doses at the first nuclear plant in the former Soviet Union*, *Appl. Radiat. Isot.* 47 (1996) 1277-1280.
- (114) KEIRIM-MARKUS, I., KLESCHENKO, E., *About adequacy of personal dosimetry data obtained by EPR signal of teeth enamel*, *Appl. Radiat. Isot.* (in press, 1999).
- (115) BOCHVAR, I., KEIRIM-MARKUS, I., KLESCHENKO, E., KUSHNEREVA, K., LEVOCHKIN, F., *New possibilities of the method of EPR dosimetry by teeth tissues*, *Appl. Radiat. Isot.* (in press, 1999).
- (116) WIESER, A., ROMAN-KO, A.A., DEGTEVA, M.O., KOZHEUROV, V.P., PETZOLD, G., *Tooth enamel as a natural dosimeter for bone seeking radionuclides*, *Appl. Radiat. Isot.* 65 (1996) 413-416.
- (117) IGNATEV, E., LYUBASHEVSKII, N SHISHIKINA, E., ROMANKHA, A., *EPR dose reconstruction for bone seeking 90Sr*, *Appl. Radiat. Isot.* (in press, 1999).
- (118) ROMANYUKHA, A.A., REGULLA D.F., *Aspects of retrospective dosimetry*, *Appl. Radiat. Isot.* 47 (1996) 1293-1297.
- (119) ZANKL, M., *Computational models employed for dose assessment in diagnostic radiology*, *Radiat. Prot. Dosim.* 49 (1993) 339-344.

- (120) CRISTY, M., ECKERMAN, K.F., *Specific Absorbed Fractions of Energy at Various Ages from Infernal Photon Sources, Part II-VII, Rep. ORNL/TM-8381/V2-V7, ORNL, Oak Ridge (1987).*
- (121) PETOUSSI-HENSS, N., ZANKL, M., *Voxel anthropomorphic models as a tool for infernal dosimetry, Radiat. Prot Dosim. 79 (1998) 415-418.*